



8D LIFE RESONANCE INFORMATION SYSTEM AURA EXPERT PRO PHYSIO[®]



LOGIN

CUSTOMIZE

EXIT

[Click here for: The ISHA Bioresonance Webshop](#)

[Click here for: The ISHA Global Bioresonance NLS and Healing Forum](#)



8D LIFE RESONANCE INFORMATION SYSTEM VIRUS EXPERT PRO PHYSIO[®]

SCREENING
MONITORING
CORRECTION
FORECAST

START

CUSTOMIZE

EXIT

[Click here for: The ISHA Bioresonance Webshop](#)

[Click here for: The ISHA Global Bioresonance NLS and Healing Forum](#)



8D LIFE RESONANCE INFORMATION SYSTEM DNA EXPERT PRO PHYSIO[®]

SCREENING
MONITORING
CORRECTION
FORECAST



Driver Version 20028
Library Version 80207

BUILD: 3.0.0.67, passed YEAR

START

CUSTOMIZE

EXIT

[Click here for: The ISHA Bioresonance Webshop](#)

[Click here for: The ISHA Global Bioresonance NLS and Healing Forum](#)

Foreword 1

This is a general basic training manual for users of

The ISHA Virus Expert Pro

The ISHA DNA Expert Pro

The ISHA AURA Commandments Pro Physio

Note:

This manual provides you basic insights in the fields of Quantum Metaphysics, Bioresonance and Non Linear Systems.

But it covers all basic functions of the programs.

For specific INDEPTH Knowledge, Secrets in Healing, Bioresonance and special functions,

Please study **The ISHA Apprentice Masters Classes**. At least the levels 1-2-3-4-5.

Then you will know it all and more than so called specialists did in 25 years.

In the classes you will also learn about:

*The special group 24 in ISHA Virus Expert Pro, select in 1 minut all disease making parasites, worms, helminth etc instead of searching for months / years.

*The selection of the more than 150+ pairs of DNA/RNA in ISHA DNA Expert Pro

*Explanations of the special AURA button and Universal Rehabilitation by The ISHA AURA Commandments Pro Physio

And you will be provided the 45 years proven to work AURA Commandments, worth 10.000, 00 and researched, tested by ISHA and a Professor from Munchen University, A Neurologist, A world famous Aura healer sir Gerhard Klugl from Lichtenstein.

Here is the link : <https://nonlinearsystem.eu/product-category/masterclass-3d8dhunter/>

ps if we wanted to make a manual like the ISHA Apprentice Masters Classes you would need a library ☺

FOREWORD 2 The Real Inventors ?

- NLS can not to be patented because it was developed by many people, scientists, organisations and companies.
- The hardware, the software, the etalons \ libraries, the in between layers of different software versions from many different healing origins, open source software packages like Borland, Delphi, and others.
- Just as we did with help of worldwide teams from Europe, Russia, China, Czech Republic, Japan, Joegoslavia, USA and many other countries.

The foundation was created by many originators of NLS, Bioresonance and Quantum Metaphysics like, Nicola Tesla, Dr. Royal Raymond Rife, Dr Hulda Clark, Voll, Niels Bohr, Einstein, Podolsky, Rosen, Gustav Kirchhoff, Ludwig Boltzmann, Michael Faraday, Heinrich Hertz, Max Planck , Max Born, Werner Heisenberg, and Wolfgang Pauli, Emil Müller, Louis de Broglie, Pascual Jordan, Erwin Schrödinger , Paul Dirac, John von Neumann, Politzer, Gross and Wilczek , Schwinger, Higgs and Goldstone, the physicists Glashow, Weinberg and Salam (and many Nobel Prize winners, not all mentioned here). And MetaGrandmaster of ISHA Who did the past 40 years 24x7

- ***A special honor is for a man and a company called www.nonlinearsystems.com**

Non Linear Systems is an electronical manufacturing company based in San Diego, California.

- Non Linear Systems was founded in 1952, by **Andrew Kay**!
- He is the true inventor of Non Linear Systems and **it all started with a simple voltmeter** ☺
- Yes, now these days YOU do already have many nonlinearsystems in and around your house ...

This company is still very well alive www.nonlinearsystems.com

- In fact **Non Linear Systems was already created NLS in 1952**, as mentioned So not by Russians, Czech's or any other !!!.
- But by sir **Andrew Kay**

All NLS software started with the use of Borland and Delphi programming. These are **open source softwares**, to be used by 1.000.000's companies. And many applications are build. Later Our factory, ISHA and others used other programming software, besides Borland and Delphi. The software and many Etalons were created with the help of many individual companies, therapists, doctors, researchers, scientists, all over the world from knowledge up to thousands of years old up till NOW . And it still goes on ... and on.

The new insights, protocols, inventions and teachings are done worldwide by MetaGrandMaster of ISHA,

- based on all knowledge going back 10 thousands of years up till now.

Catalogue

1.Introduction.....	3-9
2.Customize.....	10-19
3.NLS diagnostic and therapy.....	20-120
4.Print report.....	121-123
5.Backup.....	124-129
6.Notice.....	129
7.End.....	130

Introduction

This is a training program for use with the nonlinear diagnostic system *ISHA 8-DVA*. *ISHA 8-DVA* refers to an entirely new class of devices, which are called “brain machines” .

What are they? At present, science and society in general, is faced with information overload. Every day, there are large and small discoveries, every year there are dozens of new machines and devices developed. This is certainly good. However, a person begins to drown in this sea of information, losing the big picture.

A century ago a doctor for correct diagnosis required the experience of thousands of years of medical observation. Today this requires numerous and costly research and analysis. What helped the doctor to set the correct diagnosis? The answer is basically an inexplicable feeling called intuition.

Introduction

However, modern science has come very close to unraveling the phenomenon of intuition, and even more mysterious phenomenon of clairvoyance. The point here is that this is not a miracle or divine grace, but electromagnetic vibrations of very low frequency, which can transmit information in the human brain, bypassing the usual senses. Of the 10 million units of information only one is recognized, the others are fixed in the subconscious. Information from the sphere of the subconscious is extracted either spontaneously, or at the level of unusual, altered states of consciousness: hypnosis, dreaming, meditation, or while receiving psychotropic drugs.

The whole world, including the human race, is deeply interconnected through a variety of informational signals. That's why techniques to obtain information from the sphere of the subconscious, are recognized, while modestly, as priorities in the development of science and society in the next century.

Introduction

Numerous studies in the field of Energy-Informatics led to the creation of fundamentally new equipment capable of destroying the barrier between the conscious and the subconscious. This process (controlled research) is able to give an enormous amount of new information about the surrounding world.

A special sphere of interest - medicine. These are new opportunities for diagnosis, different from conventional ultrasound and computer tomography. An indispensable instrument for mass prophylactic examinations of the population.

Theoretical and experimental work, which made possible the development of *8D-NLS* products, was initiated in the late 19th century by electronics genius Nikola Tesla. This was then continued by George Lakhovsky, a scientist who studied the effects of radio waves on animal health and condition of plants; American researcher R. Rife, who investigated the effects on the human body not only radio, but electro-frequencies.

Introduction

In 1950, R. Voll in Russia, discovered and developed a system of electrically testing the acupuncture points of human body. Voll's method was the first hardware method of research of the energy-state of an organism. It is done by testing the rates of electromagnetic conductivity at the end points of acupuncture meridians in a person using a special probe. The results of the study (in the form of digital or graphic indicators) may give an idea of the presence of inflammatory, dystrophic or atrophic pathology in the studied meridian and the corresponding organs. Another well-known method for diagnosing the state of energy in a person - is Kirlian's aura-diagnostics . It is used to determine the state of the electromagnetic field of a human in general. Status of individual organs is determined by the configuration of their biofield. NLS-diagnostic method allows the evaluation of the state of bio-energy of each organ individually. The results can be obtained in the form of visual images with the topography of the affected area, as well as a graphical features which allow us to analyze damage to body tissue, allowing more accurately to determine not only the type of injury (inflammation or destruction), but also to clarify the diagnosis.

Introduction

Research is conducted by resonance amplification of radiation to the studied organ and then recovery of evidence via a non-contact method by using trigger sensors.

The first version of a nonlinear analysis device had only a manual input of information, that is a doctor was actively involved in the diagnosis of a patient, through the use of low frequency vibrations that are close to the theta rhythm of the brain becomes more sensitive to radiation in the body of the patient. The results were recorded using the deviation of an L-shaped frame held by the physician-operator on Flanders' s special scale (this scale is presented in the diagnostic module of the program). However, this method of research is too subjective and not safe for the health of the physician operator. This led to the development and creation of so-called trigger sensor, providing automatic input of information about the health of the patient in the computer. On what is the effect of trigger sensors?

Introduction

For the first time a distant effect of interaction with objects of animate and inanimate nature, that is the transfer of data pulses from a man to machine was registered in the experiments of V.N. Kravkov in the 20-ies of our century. Under the guidance of prof. V. Togatova, reactions of various semiconductor structures on the impact of bio-operators (psychic), were studied. It has been experimentally proved that the human brain without the aid of wires can have an affect the sensitive sensor device.

Software developers, in a dialogue mode between the telemetry complex and the physician operator with remote biofeedback, designed for the perception of the brain activity of the operator or patient but depending on the objectives of the study and configuration of the complex and convert this information into a sequence of pulses with a special trigger sensor. This is reflected in the fact that the human brain receives a signal about the need to verify (test) this or that organ. The signal is fed to the monitor screen, as well as the head headphones in a series of electromagnetic waves peculiar to the healthy human body. This is possible because every organ and every cell in the human body has its own spectrum of electromagnetic waves. Thus we would like to ask the question - what is going on with the target organ? In response to the question, the brain of the subject gives an answer that is perceived by the trigger sensors.

Introduction

In the model, the «ISHA 8-DVA» device offers a digital trigger sensor, simulated directly in the microprocessor of the main unit through the computer software and analog trigger sensor of the main research unit - pn-junction transistor, which increases the reliability of research.

The purpose of this training program is not a detailed physical justification of the principles of the «ISHA 8-DVA» device, since different devices are designed differently. Currently, there are several manufacturers of this equipment, “spinoffs” from the original research group. In particular, in the original version of Russian, the headphones were used as magneto-inductors with an oscillation frequency, which is close to the thetarhythm of the brain, while in later versions of the device - as a conductor of electromagnetic waves that are close to the alpha rhythm of the brain. A good effect is obtained from the use of electromagnetic waves as a trigger mechanism for the study of a healthy body. Also, in many other versions of the device, laser emitters are used to affect the brain of the patient. Using the laser leads to an increase of the resonant response. However, there is a risk of adverse effects of such exposure, so the laser emitter is not used in all models of *ISHA 8-DVA* equipment.

Customize

Click the "**CUSTOMIZE**" button (Fig.2).

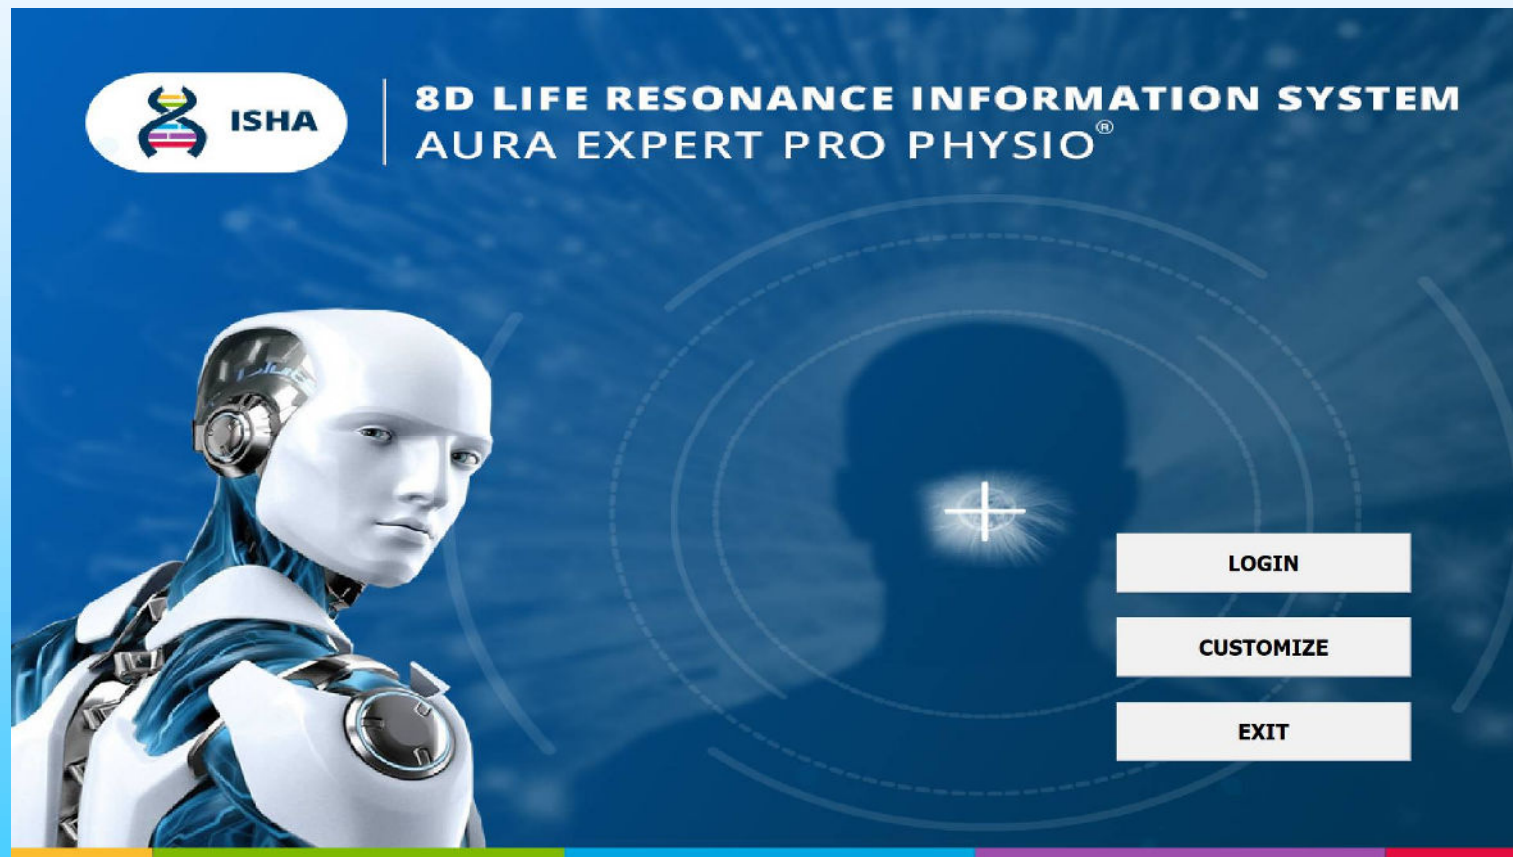


Fig.2.

Customize

Settings menu(Fig.3).

The screenshot shows a software settings window with a light blue background and a grey border. At the top left, there are two buttons: "Select doctor" and "Administrator". At the top right is an "EXIT" button. Below these, the window is divided into two main sections. The left section is titled "Language" and contains a list box with "English" selected. The right section is titled "Speed" and contains a list box with "Very fast" selected. Below the "Speed" list box, there are four buttons arranged in a 2x2 grid: "Bold font", "Color in card-index", "Color images", and "Enable sound".

Section	Option
Language	English
Speed	Very fast
Speed	Fast
Speed	Medium
Speed	Slow
Speed	Very Slow

Buttons: Select doctor, Administrator, EXIT, Bold font, Color in card-index, Color images, Enable sound.

Fig.3.

Customize

Select doctor : allow to choose a doctor from the list of doctors working with the device. Each doctor can see only his/her own patients and can not see patients of other doctors.

Administrator : open administrator panel.

Language : change the language of the program. The base version of the program is delivered in English.

Exit : allow to return to the main menu.

Speed : change to different model.

Customize

Bold font : show all the text in bold.

Color images : can see colorized pictures of organs in the research scheme.
If this button is clicked off the pictures are in black-and-white.

Color in Card-index : allow to highlight automatically in different colors of the organs with various functional statuses in a card file after researching.

Green marks organs without the expressed functional changes.

Red is for organs with insignificant functional changes.

Brown is for organs with considerable functional changes.

Enable sound : switch on sound signals when the device is working.

Customize

The button '**Administrator**' allows the owner into a administrator model.
(Fig.4.)

The screenshot shows a software interface titled "Doctor". At the top, there are two buttons: "Delete research" and "Exit". Below "Delete research" is a table with two columns: "Date" and "Title Research". The table is currently empty. To the right of this table is a vertical stack of buttons: "Record fees", "Patient exchange", "Doctor selection", "Report", "Delete by date", and "Delete card file". Below these buttons is a "Search" label followed by a text input field. At the bottom of the interface is a larger table with seven columns: "Last name", "First name", "Middle name", "Age", "Sex", "Address", and "Phone". This table is also empty.

Fig.4.

Customize

Delete research : allows to delete separate researches with the button, located at the top of the window.

Patient Exchange : allows to transfer a patient to any other doctors from this list. Since this moment only the new doctor will be able to see information about the patient.

Doctor selection : allows to add a new doctor or to delete a doctor from the list. Attention! If you delete a doctor from the list of doctors, all data of the patients treated by this doctor is deleted as well. Therefore before removal, pass all patients of that deleted doctor to the other one. The given button also allows to choose the doctor from the list for current work.

Report : shows many researches carried out by each doctor or by all doctors together.

Customize

Delete by date - allow to delete all researches of a specified date.

For example, a year to the present date, all previous researches made before this date will be deleted.

Delete card file - allow to delete a patient from a card file.

Customize

Patient exchange

Each doctor in the program can see only his/her own patients and can not see patients of other doctors. If it is necessary for the administrator to delete one or several doctors from the list, their patients and all data will be deleted together with the deletion of these doctors. If it is necessary for you to save data of these patients, please transfer their data to other doctors whom you are not going to delete before removal of doctors from the base(Fig.5)

The interface displays two side-by-side lists of doctors. The left list contains 'Doctor', 'Doctor2', and 'Doctor3'. The right list also contains 'Doctor', 'Doctor2', and 'Doctor3'. Between the lists are three buttons: 'EXIT', 'Move card file', and 'Single ->'. Below these buttons is an 'All ==>' button. At the bottom, there is a table with columns for 'Last name', 'First name', 'Middle name', 'Age', 'Sex', 'Address', and 'Phone'. The 'Last name' column has a text input field below it.

Last name	First name	Middle name	Age	Sex	Address	Phone

Fig.5.

Customize

Choose the doctor in the left top corner of the screen, WHOSE patients should be transferred to other doctor. In the right top corner of the screen choose the doctor WHO should receive the patient.

Then choose the patient whose data you wish to transfer and click **Single ->** or click **All=>>** .

You also can choose another patient and transfer his/her data further (Fig.6).

Be attentive as the data are transferred not copied!

After that, you can return to the administrator's panel using the “**Exit**” button.

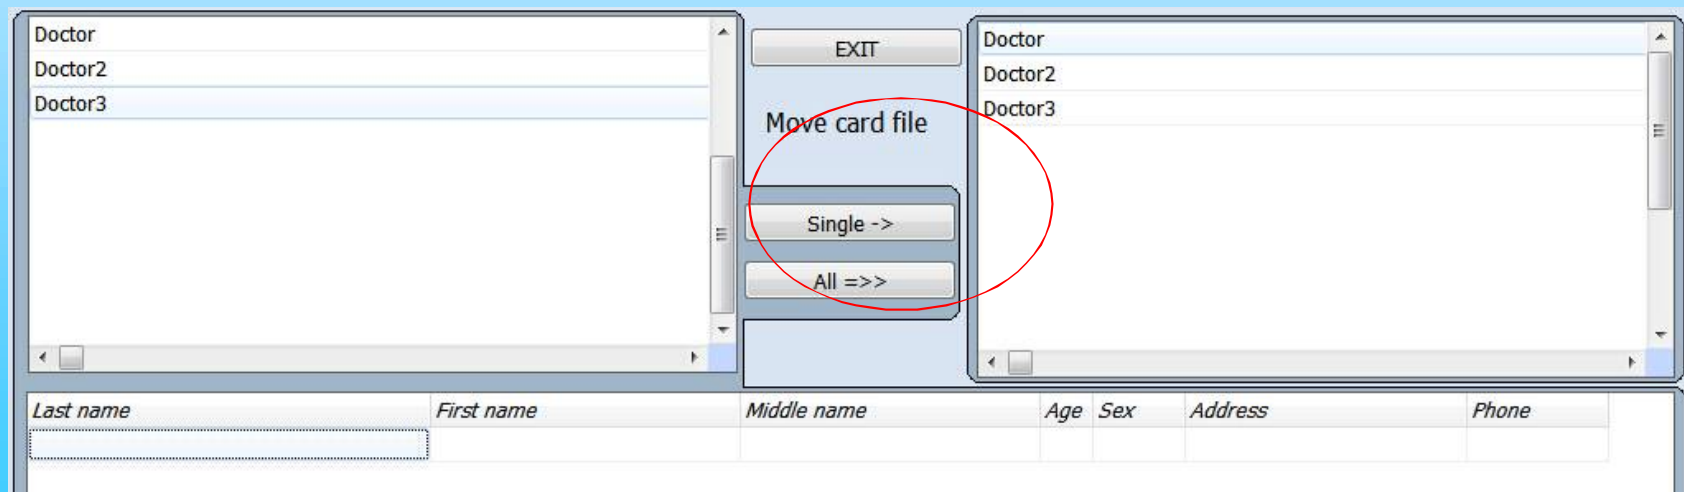


Fig.6.

NLS diagnostic and therapy

Click the '**LOGIN**', it will show user the Card Index (Fig.7)

The screenshot displays the 'Card Index' interface of the NLS diagnostic and therapy software. The interface is divided into several sections:

- Top Left:** A form for patient information with fields for Last name, Name, Middle name, Age, Sex, Blood group, Address, and Phone.
- Top Center:** A 'Search' field and an 'EXIT' button.
- Top Right:** Three buttons: 'Delete by date', 'Delete research', and 'Delete file card'.
- Below Top Left:** Two buttons: 'New card' and 'Select card'.
- Below Top Center:** A 'Reception by Doctor' field.
- Below Top Right:** A large, empty rectangular area.
- Bottom Left:** A table with two columns: 'Date' and 'Name of research'. The table is currently empty. Below the table is a status bar showing '0/0'.
- Bottom Center:** Three buttons: 'Print epicrisis', 'Save to disk', and 'Print researches'.
- Bottom Right:** Three buttons: 'RESEARCH', 'View result', and 'Comparative analysis'.

Fig.7.

NLS diagnostic and therapy

New card : allows to input a new patient.

Select card : allows to choose a card of a client from the list. If you click this button, you will see the list of clients treated by the given doctor. About each client the following information will be accessible: first name, middle name, last name, age, sex, address, phone number.

Print epicrisis : allows to print all the data chosen by the doctor (results of research, comments of the doctor).

Save to disk : allows to save the data of the client on a CD or a hard disk and to transfer them if necessary to the other computer.

Print research : allows to print the latest research of a patient. The program allows to print out 4 pictures with 100*100 mm size in A4 paper.

NLS diagnostic and therapy

Research : shows the research scheme (or the interactive anamnesis if you click this button for the first time for a new patient).

View result (when the headphones are off) or **Current analysis** (when the headphones are on the client's head) allows viewing of research results.

Comparative analysis : allows to make comparison of researches conducted at various times or under different conditions for the same patient to study the dynamics of virtual testing standards or Meta-therapy influence.

Graphic : it is under a picture of the examined organ or system you will see the diagram of spectral similarity of etalon processes.

NLS diagnostic and therapy

Delete by date - all researches done before this date will be deleted.

Delete research - delete selected research.

Delete file card - delete the patient card at present.

Search Text - search the patient all researches record. For example, input the patient name: Ken, in the bottom part of the screen will show "Ken" all researches record.

NLS diagnostic and therapy

Click the '**New Card**', and filling all the blanks, it will turn to the next page.(Fig.8)

The screenshot displays the NLS diagnostic and therapy software interface. A 'New Card' dialog box is open, allowing users to enter patient information. The dialog box contains the following fields:


- Last Name
- First name
- Middle name
- Birthday (with a dropdown menu showing '1900/ 1/ 1')
- Age
- Sex
- Group of blood
- Resus Phactor
- Address
- Phone
- Handy
- E-mail

At the bottom of the dialog box are 'OK' and 'Cancel' buttons. The background window shows a 'Last name' field, a 'Search' field, and an 'EXIT' button. Below these are buttons for 'Delete by date', 'Delete research', and 'Delete file card'. A 'Reception by Doctor' section is also visible. At the bottom of the background window are buttons for 'RESEARCH', 'View result', and 'Comparative analysis'. A 'Print epicrisis' button is located near the bottom left of the background window. The bottom left corner of the background window shows '0/0'.

Fig.8.

NLS diagnostic and therapy

This is a location to point out health history for doctors, and a location allowing for the patient to provide more interaction to the therapist, thus allowing them to express areas of concern that they wish the technician to know about. (Fig.9.)

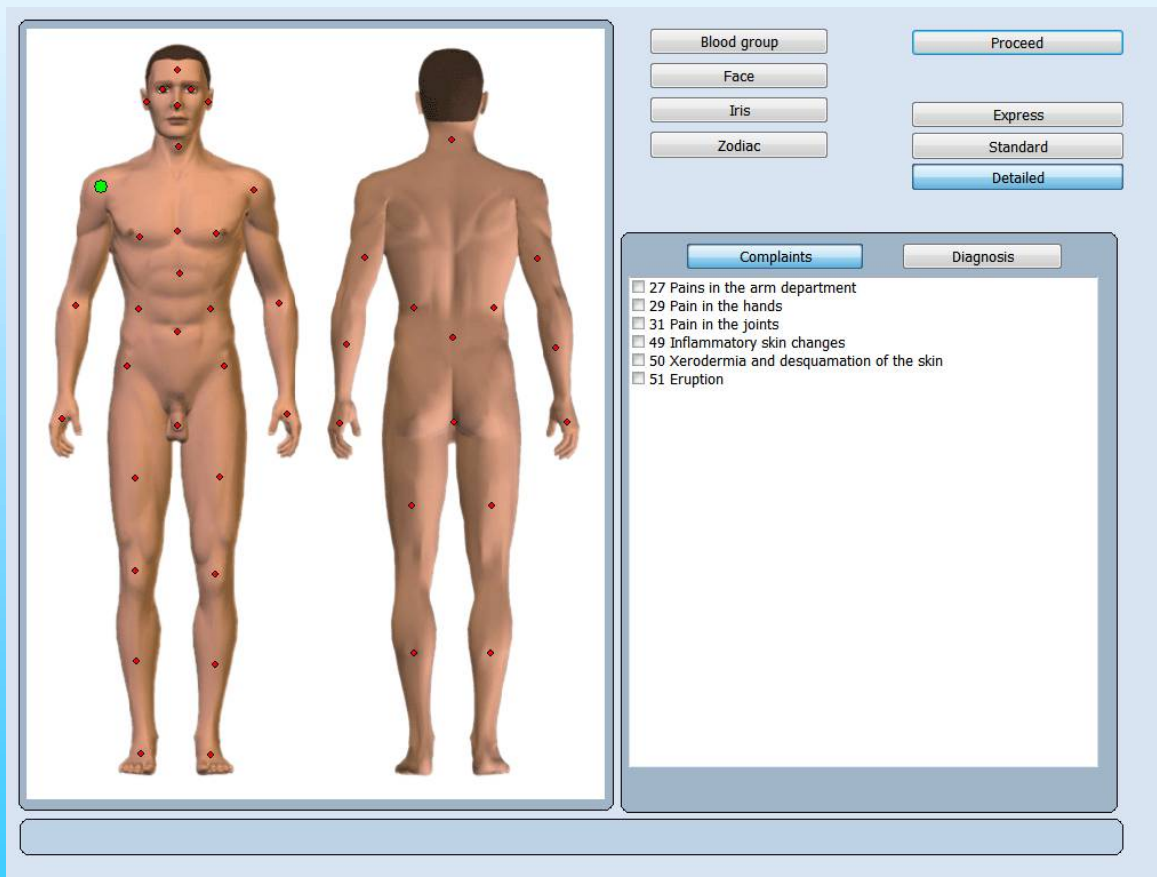

You will notice that the right shoulder has the green dot on it to start. Once you click the area you want you click on as many of the list of the right as you wish that are pertinent, you will see the dots change from green to red as you choose them. After this you can click on another area of the body.

Fig.9.

NLS diagnostic and therapy

This mode is accessible only once after registration of a new patient. The interactive anamnesis is intended for active participation of a client in the course of data gathering by a doctor to receive extensive information on complaints and diagnoses of the patient during their dialogue. It allows to come into more friendly contact for a period of examination as it is very important for any doctor.

Using dynamic points, the doctor can input the data about diagnoses and diseases known to the patient. It will help later to make integrated and reliable analysis of the examination results.

The investigation scheme

This menu allows a doctor to prepare the device for carrying out the investigation (research) by choosing type, speed, necessary organs and other important parameters

NLS diagnostic and therapy

Complaint: Offers the choice by issue of patients. (Fig.10)

Diagnosis: Offers the list by predetermined medical diagnostic complaints. (Fig.11)

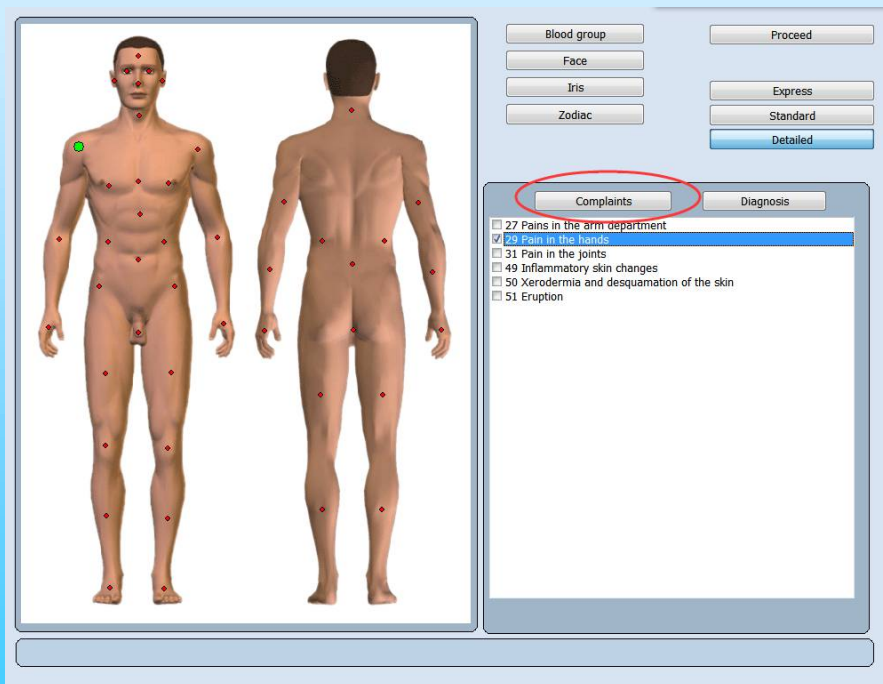


Fig.10.

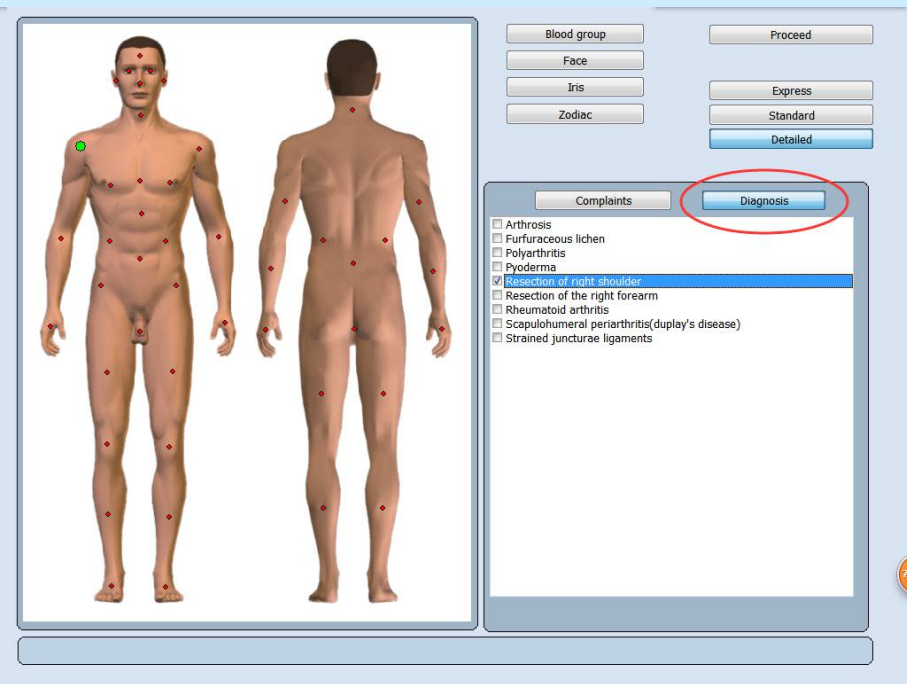


Fig.11.

NLS diagnostic and therapy

Express: allows to carry the general analysis without detailed investigation.

Normal: allows to carry the general analysis without detailed investigation, but with more detailed examination of biological structures with the expressed functional changes.


Detail: allows to estimate in details each biological structure from the list and investigation takes quite a long time.

Proceed : can go on the next step.

NLS diagnostic and therapy

Blood Group, Face, Iris, Zodiac, show you some reference. (Fig.12)

Blood
Group

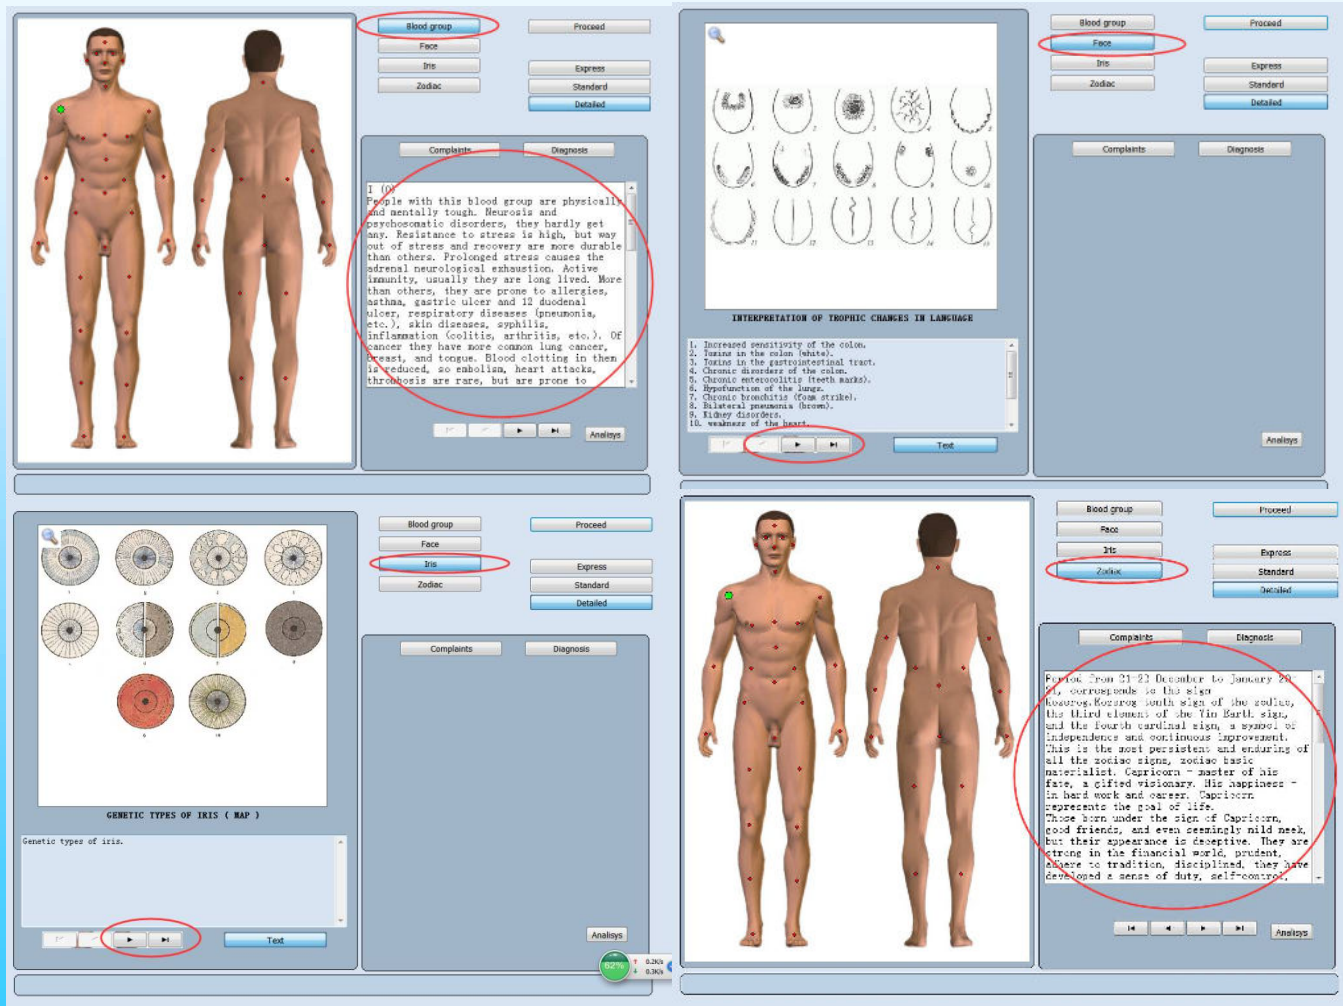

Face

Fig.12

Iris

Zodiac

NLS diagnostic and therapy

Click the '**Proceed**', it will show you this page Scheme of investigation. (Fig.13)

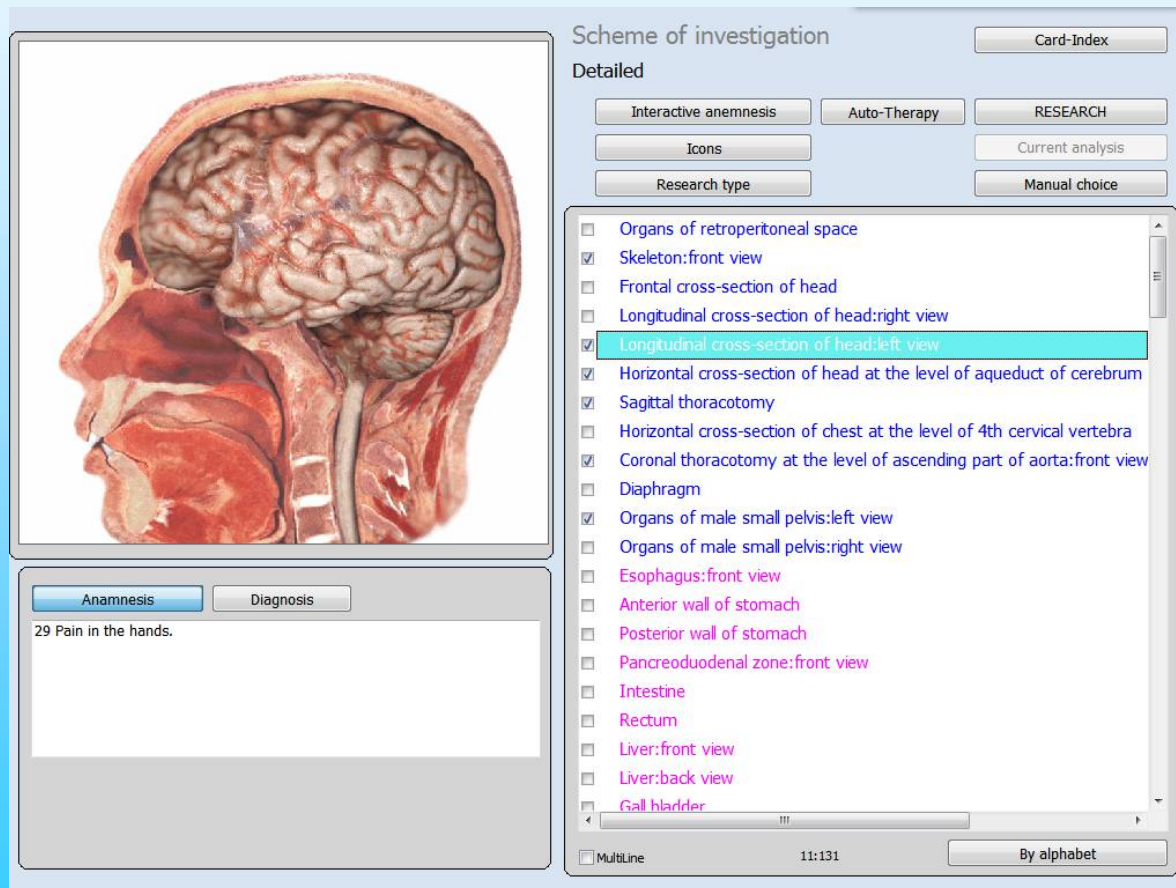


Fig.13

NLS diagnostic and therapy

Card index : allows to exit the scheme of investigation and return back to card file.

Anamnesis: show you complaints of patients.


Diagnosis : show you diagnoses of doctors.

Interactive anamnesis : can return to Interactive anamnesis main menu (Fig.13)

Auto-therapy : need to choose has the investigation organ or tissue or cell. Under the window you can see a window with a picture of the selected organ from lists of organs, tissues, cells (Fig.13).

Icons : show more detailed examination of the organ (Fig.14). You will see a set of icons on the picture of the organ, showing other organs systems and tissues connected with it.

Fig.14.

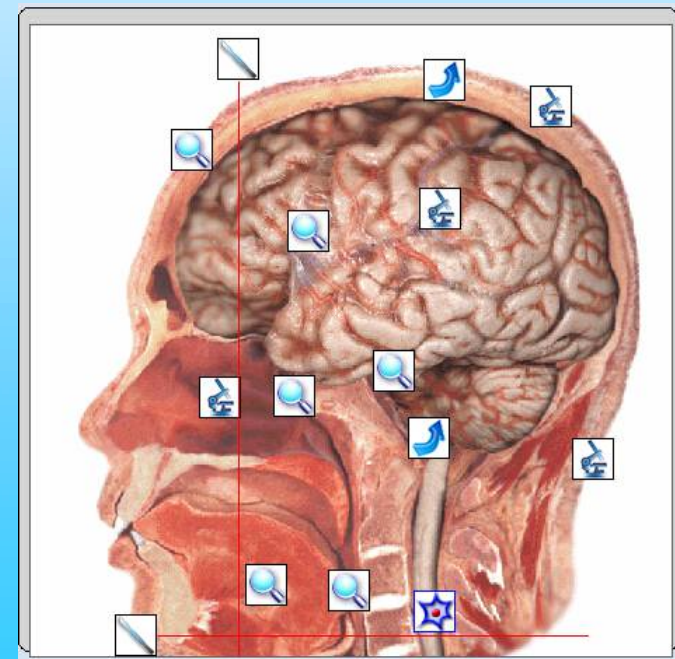

NLS diagnostic and therapy

Icons are divided into several types:

Icons with images of cells allow to carry examination of cells of this organ. 

Icons with the microscope or magnifier image represent tissues, groups of cells, profiles and parts of the chosen organs or system. 

Icons with the image of an arrow denote the systems connected with given organ and other organs. 

Icons with the magnifier image allow to conduct a more detailed research of this area. 

The Virtual scalpel allows to investigate the given organ or system in a different profile. 

NLS diagnostic and therapy

Research type

Express : allows to carry the general analysis without detailed investigation.

Normal : allows to carry the general analysis without detailed investigation, but with more detailed examination of biological structures with the expressed functional changes.

Detailed : allows to estimate in details each biological structure from the list and investigation takes quite a long time.

Science : allows to show all the organs list.

Research : allows to begin investigation with the set-up parameters under a set-up scheme of investigation from the list of organs.

Current analysis : opens the menu of the current analysis described further

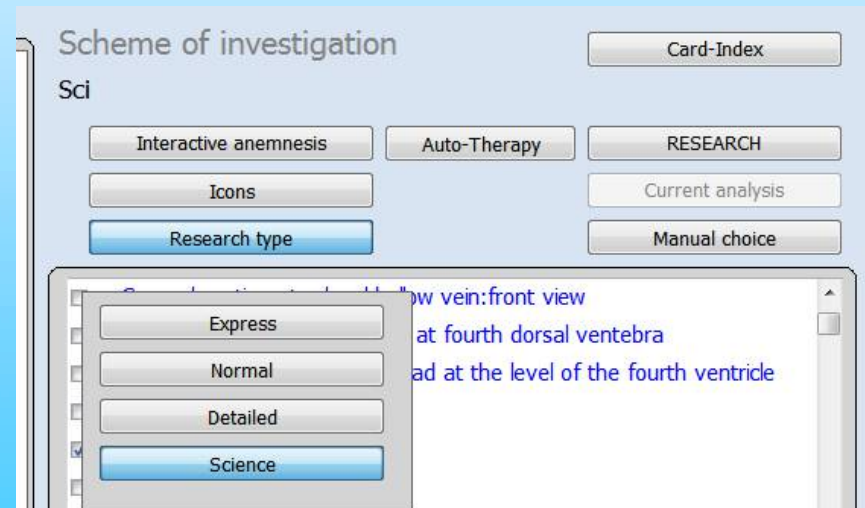


Fig.15.

NLS diagnostic and therapy

Click '**Manual choice**', it will show you some choices.(Fig.16.)

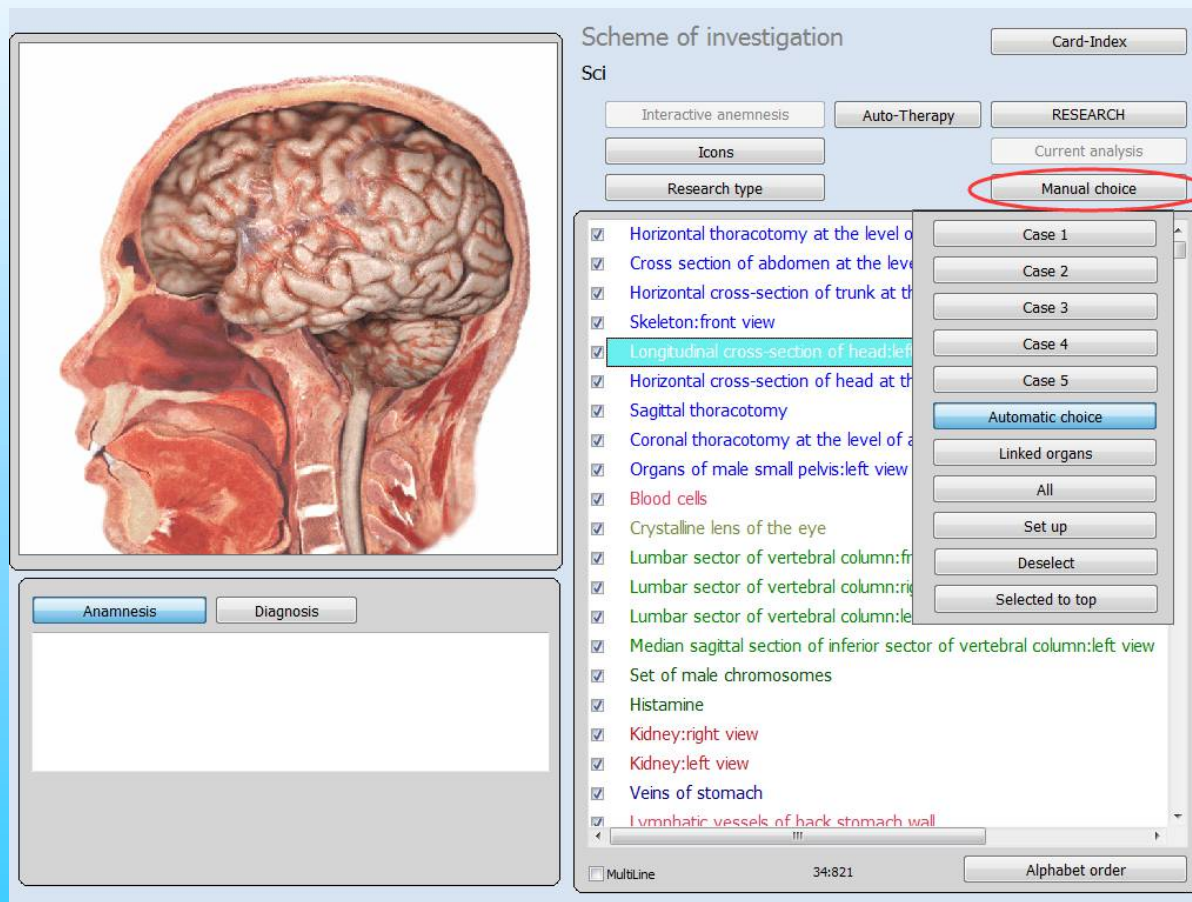


Fig.16.

NLS diagnostic and therapy

Manual choice : you can click on a small square to the left of the organ from the list and it will be automatically added to the investigation scheme. To remove any organ from the investigation list click on it once again. (Fig.18.)

Automatic choice : the computer will offer you a number of basic systems and organs of a body from the list of all investigations. We recommend to use this mode for primary examination of each new patient.

Case 1, Case 2, Case 3, Case 4 Case 5 : It is the custom investigations scheme.

Linked organs : choose some linked organs to research automatically.

All : it is chosen all organs from the investigation list.

Set up : it is custom the case1, case 2, case 3, case 4 ans case 5 investigations a new choice for disease in advance.

Deselect : deletes all chosen organs from the investigation list.

Selected to top : make all the organs be choosed to the top.

System order and alphabetically **Alphabet order** make organs can be sorted out by systems.

Multiline : show pictures of the organs. (Fig.17.)

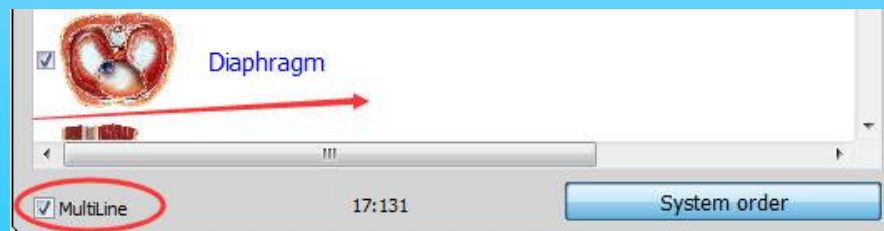


Fig.17.

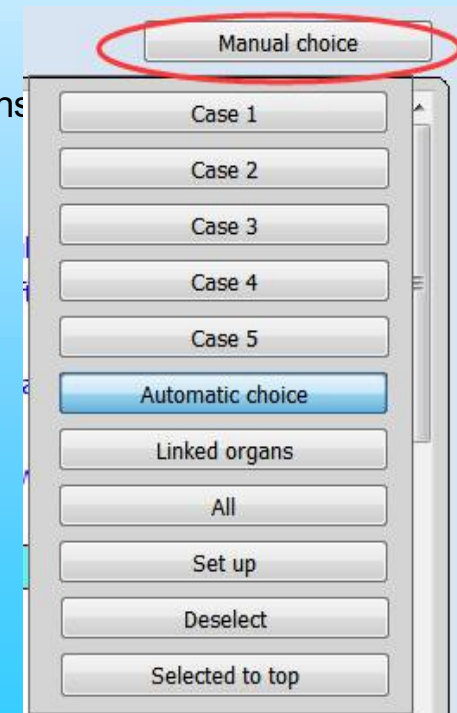


Fig.18.

NLS diagnostic and therapy

- ☐ TRANSVERSAL SECTION OF RACHIS in cervical zone
- ☐ TRANSVERSAL SECTION OF RACHIS in thoracic zone
- ☐ TRANSVERSAL SECTION OF RACHIS in lumbar zone
- ☐ MIDSAGITTAL CROSS-SECTION OF BODIES OF VERT
- ☐ LONGITUDINAL SECTION OF RIGHT KIDNEY
- ☐ LONGITUDINAL SECTION OF LEFT KIDNEY
- ☐ KIDNEY; right V
- ☐ KIDNEY; left V
- ☐ NEPHRON #
- ☐ GLOMERULES AND INCOMING ARTERIES
- ☐ ARTERIES OF HEAD AND NECK; right side
- ☐ ARTERIES OF HEAD AND NECK; left side
- ☐ On the right of the heart
- ☐ On the left of the heart
- ☐ MUCOSA OF NASAL CAVITY # MK
- ☐ TRACHEA AND BRONCHI
- ☐ CORONAL CROSS-SECTION OF LARYNX AND TRACHEA
- ☐ TRANSVERSAL SECTION OF LARYNX # MK
- ☐ CROSS - SECTION OF NECK

In the investigation scheme all organs, cells and tissues are sorted according to the systems(Fig.19), for example: blue color marks systems of organs and sections of the interior of human body, green is for bone system etc. In the list of organs sorted by systems, you can see names of cells which are marked with a different color but belong to the given systems.

Interactive anamnesis allows to enter the menu of the interactive anamnesis before the first examination of a patient to specify complaints and diseases.

Fig.19.

Click the ' **Research** ', it will work automatically.(Fig.20.)

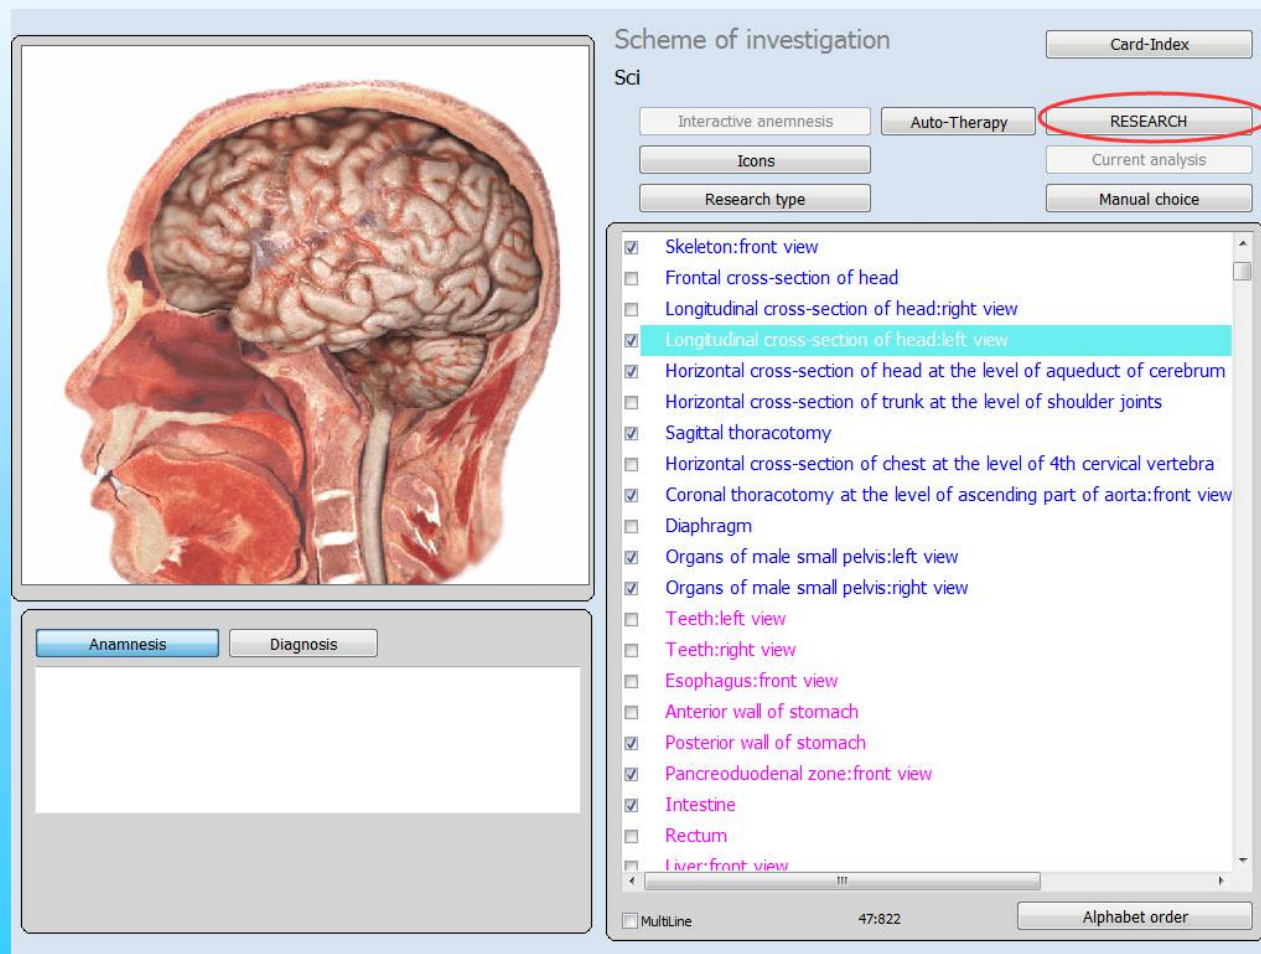


Fig.20.

NLS diagnostic and therapy

Research procedure

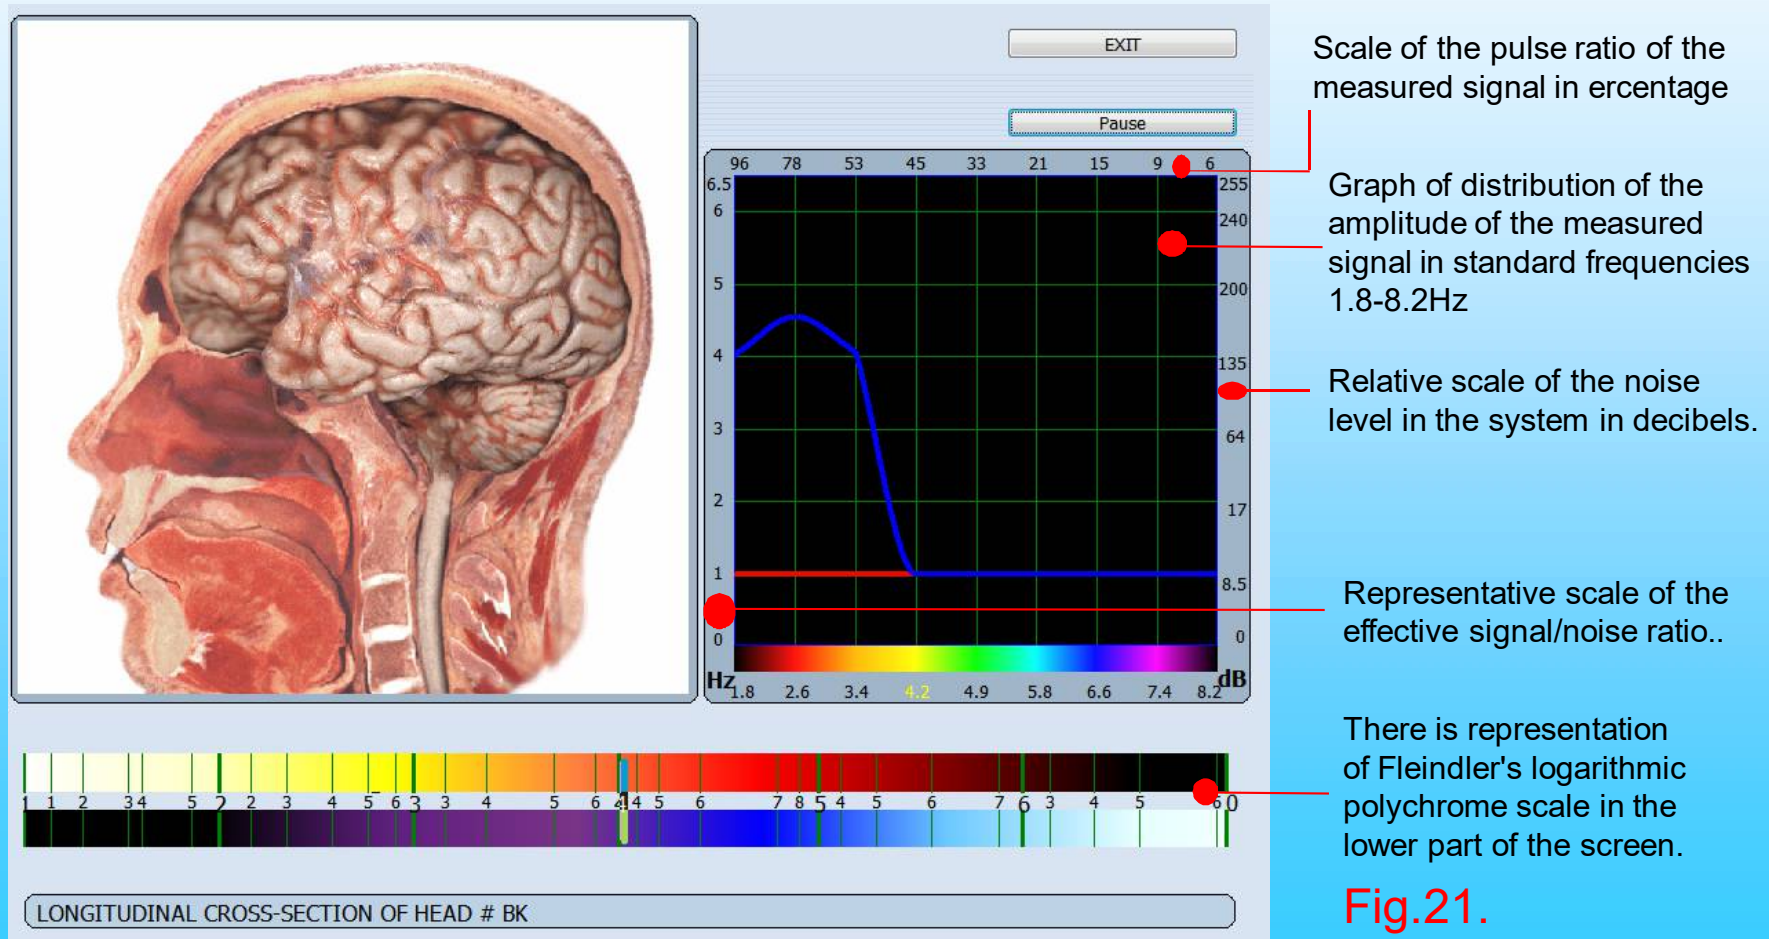


Fig.21.

NLS diagnostic and therapy

Pause/Resume : allows to make a pause in a research if necessary. You also can remove the headphones during the research and it will be automatically stopped until you put them on again.

Exit : allows to return to a card file.

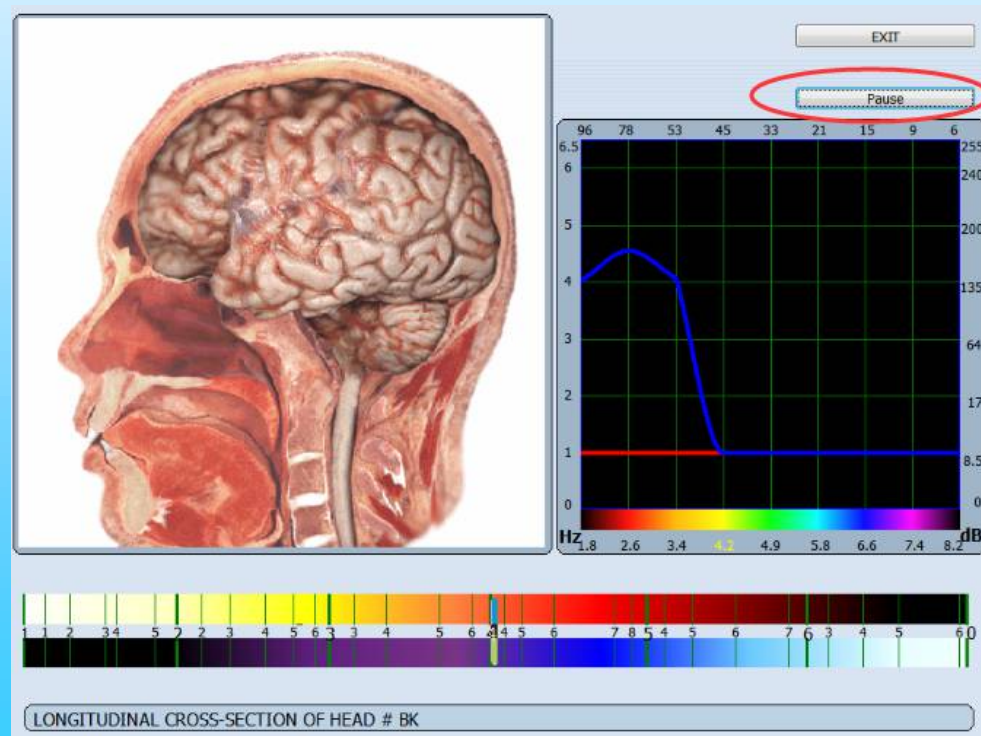


Fig.22.

NLS diagnostic and therapy

Control points, levels and curves

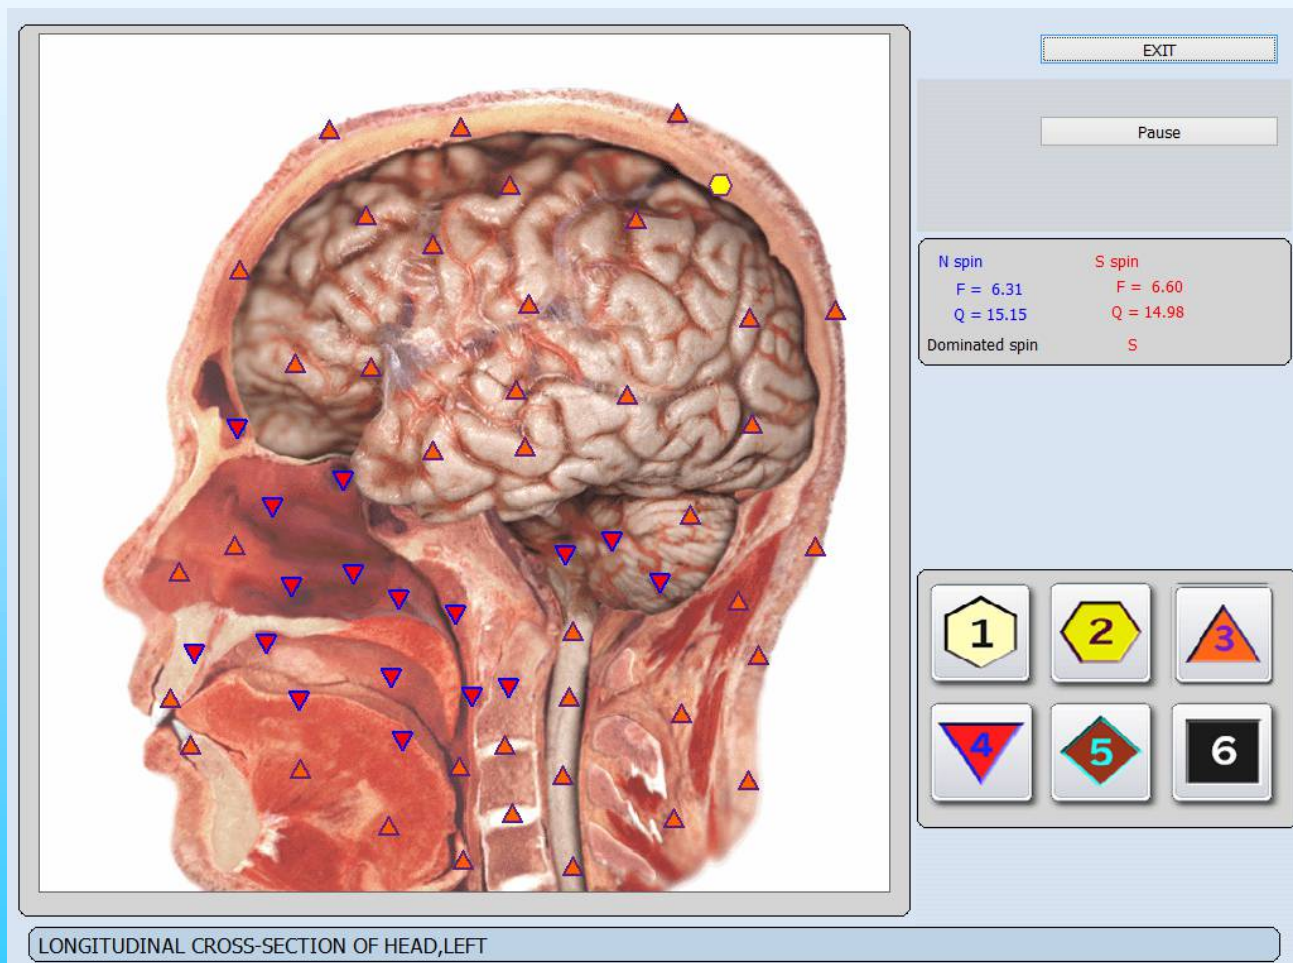


Fig.23.

NLS diagnostic and therapy

'Research' mode allows to compare the received signals from the head-phones to the etalons. The results are presented on the Flendler's scale.

6 various icons designating the following levels(Fig.23):



lower limit of normal



mild changes (pre-clinical stage of disease)



standard



change of the average degree (clinical stage of disease)



upper limit of normal
(transition state, the functional changes)



pronounced changes

NLS diagnostic and therapy

It is VERY IMPORTANT! Since the method of nonlinear analysis refers to the energy techniques, visual assessment of damage to the body belongs to the state of his energy!

In most cases correspond to the somatic energy damage, but there are cases where power failures precede the development of somatic disorders. In these cases, the state body may be observed in black squares. In the analysis of such situations, the smallest QRS is most often a organopreparations (that is, a healthy body).

The present model was designed with possibility of simultaneous analysis of several data channels. It allows to carry out the analysis of signals in control points with very high speed.

It is important to remember that the given scale of levels is approximate and serves mainly for evaluation of adaptive capability of an organism (strengthening, weakening). Even the strongly pronounced divergence cannot unequivocally be interpreted as disease without preliminary estimations and comparisons.

During the examination you can evaluate conditions and reserves of an organism of the client at the specific moment of time.

NLS diagnostic and therapy

For example, if your patient has no serious illnesses but has a serious depression at the moment, non-regular meals, sleep, work a lot with the computer, you can see a lot of 4,5,6 levels in control points during the examination. Thus you cannot draw a conclusion on the presence of any diseases.

Another case: your patient has a number of chronic illnesses out of the aggravation period, thus basically you see levels 1, 2, 3. It can mean that the patient has the right treatment, medicines and his organism has good reserves.

A different case: the client's appendicitis or any other organ is cut out. When examining this organ the computer gives out mainly levels 1,2 or levels 5, 6 and it means that the device does not know how to conduct the survey in this case as the organ is already not present and the brain continues to send signals to this organ (phantom effect).

NLS diagnostic and therapy

Card file of the client after research

Last nameTom

NameR

Middle name

Age38Sex Male

Blood group: 00

Address

Phone

Search

EXIT

Delete by dateDelete researchDelete file card

15:52:02


Reception by Doctor

Time 15:52/0:00

New CardSelect Card

Print epicrisisSave to diskPrint research

Date	Name of research
03.06.2014	LONGITUDINAL CROSS-SECTION OF HEAD # BK
03.06.2014	HORIZONTAL CROSS-SECTION OF HEAD at the level of aqueduct of cerebrum
03.06.2014	HORIZONTAL CROSS-SECTION OF HEAD at the level of the fourth ventricle
03.06.2014	CORONAL THORACOTOMY at the level of ascending part of aorta, front view
03.06.2014	CORONAL THORACOTOMY at the level of venae cava, front view

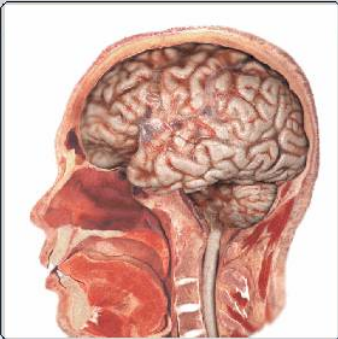

Graphic

RESEARCH

Current analysis

Comparative analysis

Fig.24.

NLS diagnostic and therapy

If the research is finished you can go back to the patients card file.(Fig. 30) and go through the list of examined organs at the bottom of the screen. You can choose any organ from the list for the comparative analysis and the further researches.

You can sort researches by date or alphabetically when you click the mouse on heading of date or research name twice.

The current analysis/viewing of results

If the research is finished you can open following menu (Fig.31) if you click the button View result/Current analysis.


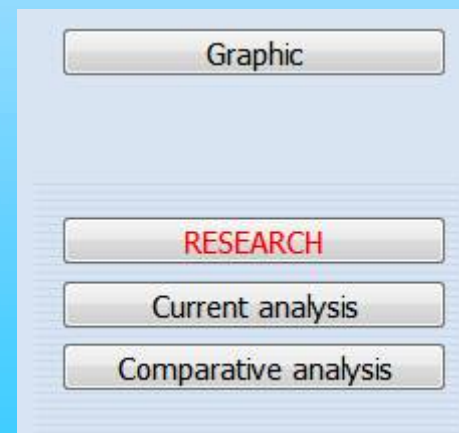


Fig.25.

NLS diagnostic and therapy

Investigation icon

In the investigation list, shows investigation organ records, the investigation icon represents the following meaning(Fig.26):

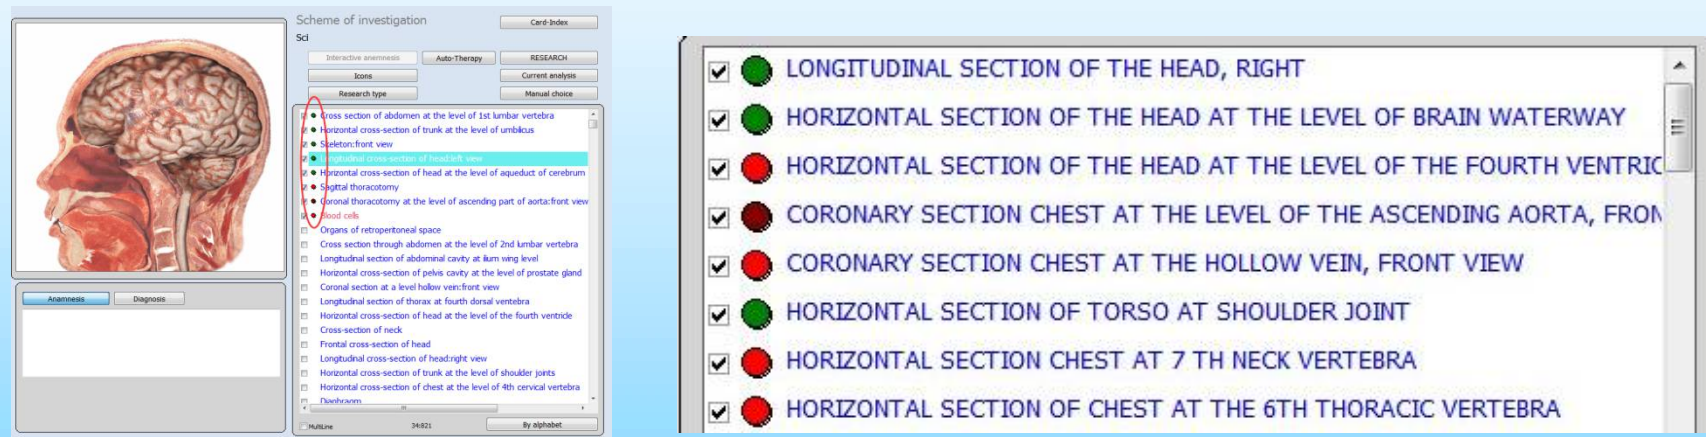


-  Means the organ generally good
-  Means the organs slightly dysfunction
-  The organ beneath subordinated parts

Fig.26.

This is just a preliminary analysis of the disease development trend ,You need to confirm by **Entropy Analysis** and **NLS - Analysis**.

NLS diagnostic and therapy

After 'research done', Click the '**Current analysis**'

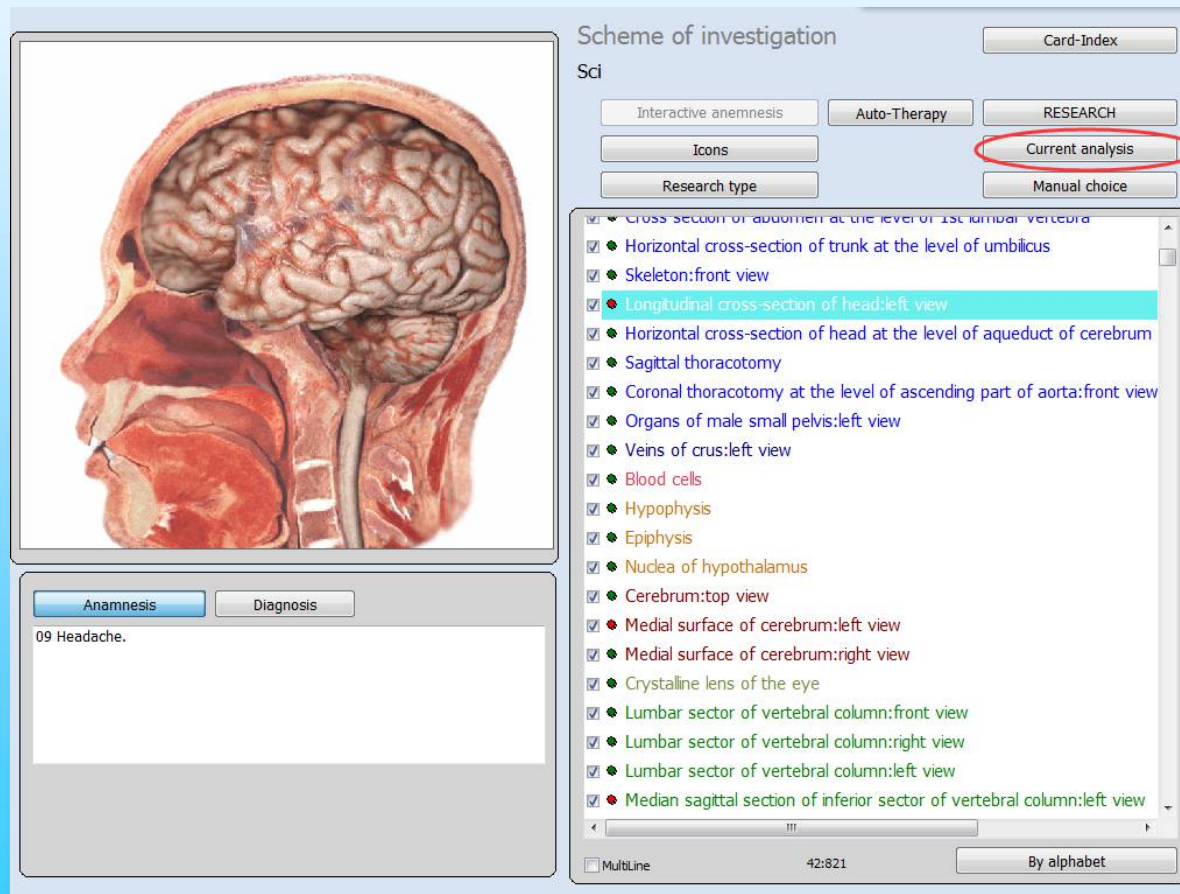

Choose these
two color dots
to analysis

Fig.27.

NLS diagnostic and therapy

It will appear this page, know these buttons function first.

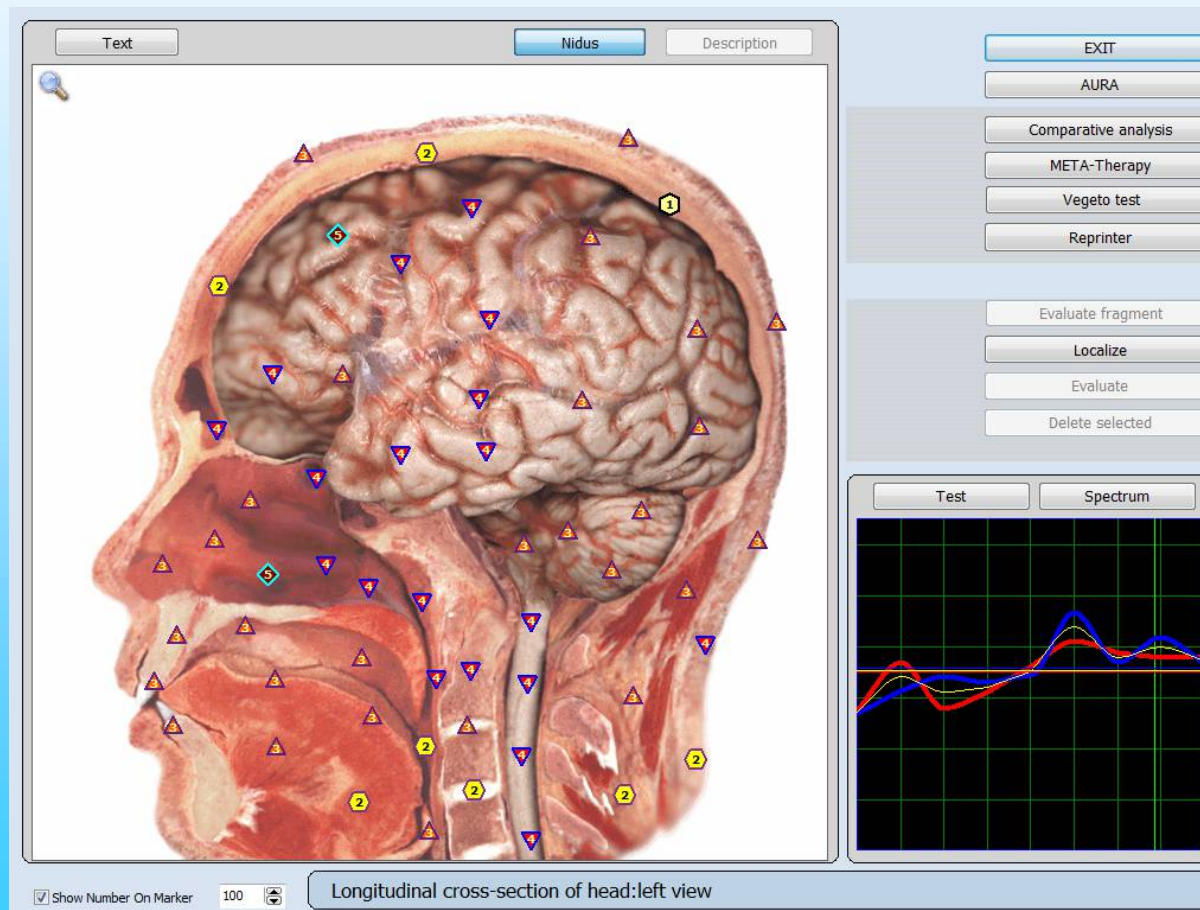


Fig.28.

NLS diagnostic and therapy

Eixt : Allow to back to scheme of investigation (previous page)

AURA: the electromagnetic field that surrounds every living being and is manifested in the physical field by electrically charged objects that represent themselves as different colors that surround the body. This electromagnetic field can provide information regarding a person's emotional state, the quality of consciousness and will determine the level of health regarding an individual organ and organ systems.

Comparative analysis: To make a comparative analysis of research of one organ made at various times or under different conditions.

META-therapy: (classical bioresonant therapy), see next chapter.

Vegeto test: (external), To evaluate reference data, see next chapter.

Reprinter: To put down the information about the reference data (etalons) into the matrix: Water, Alcohol, Sugar, Paraffin.

Localize and Evaluate: To allocate area and to estimate, allows to allocate a part of an organ and to evaluate it. It is necessary to notice that the less allocated area and the more

difficult the form of borders of allocation, the less exact results of the analysis. Therefore it is recommended to choose an organ or a cell corresponding to the area of interest from the list of organs or to carry out the comparative analysis of testing results of adjacent organs and systems, to collect the more informations from the patient.

Evaluate fragment : Enable to make a more thorough evaluation of the marked area on the organ projection in the scaling mode.

Delete selected: To delete allocate area.

Test : To enter the reference data menu.

Spectrum : To see the curves of signals of a larger size.

NLS diagnostic and therapy

Text : show you green crosses on the picture of an organ. If you select any of the crosses with the cursor you will see in pop-up menu the help information in the form of the name of an organ which specifies the given green cross.(Fig.29)

All text : show you all the help you information(Fig.30).

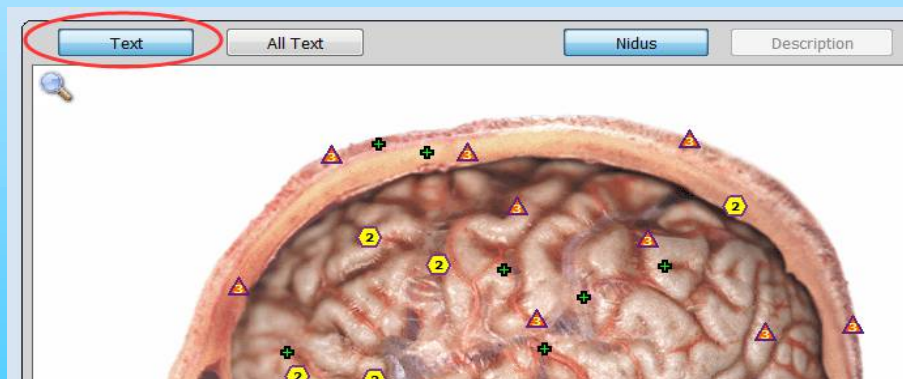


Fig.29.

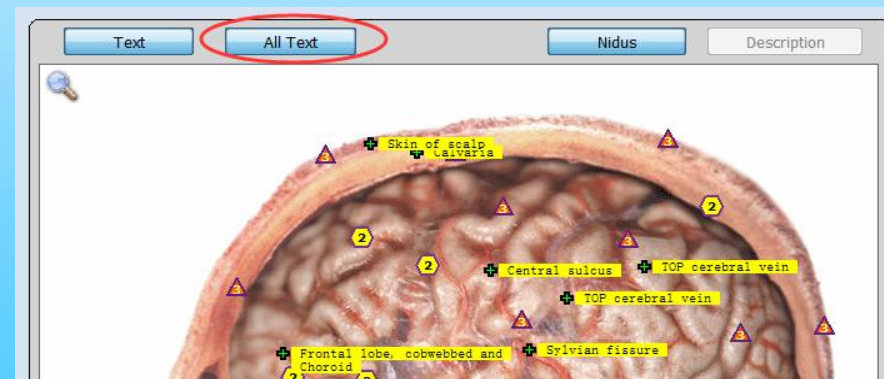


Fig.30.

NLS diagnostic and therapy

Description : enables to give a description of the biological object shown in the picture.

Nidus : allows to show/hide the localisations of the given organ designated by the doctor. You also can show/hide them by clicking on the left button of the mouse.

If you click the icon  on a magnifier in the left top corner of the screen it is possible to enlarge the selected image with the click of the mouse. if you click  returns the picture to its initial size.

NLS diagnostic and therapy

The Treatment with META-Therapy

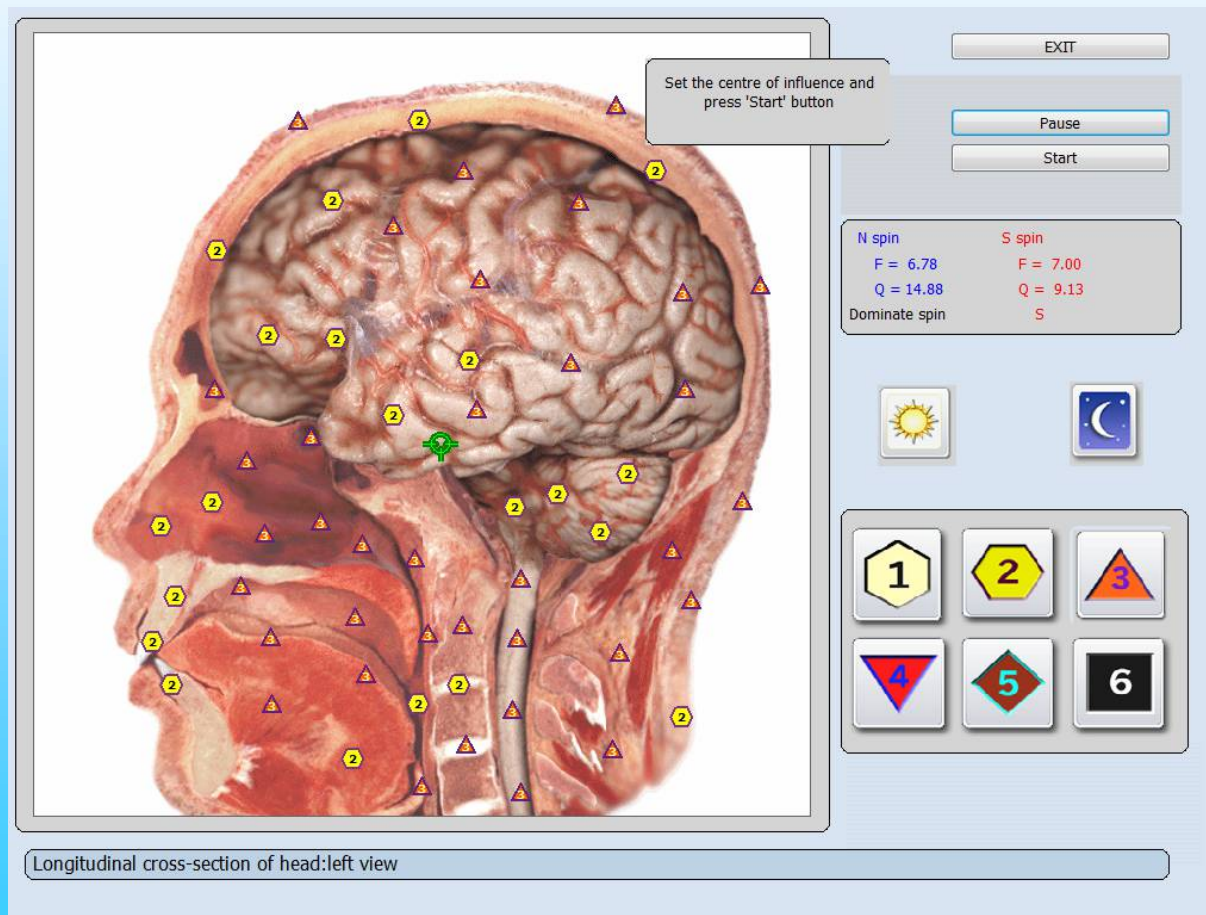


Fig.31.

NLS diagnostic and therapy


Einstein Said: "Everything in life is Vibration."

There are many things between heaven and earth that cannot be explained by University or Physical science, although they do exist, no doubt!

Bio-Resonance Feedback Therapy (META-Therapy) is a frontier technology based on quantum physics. Bio-Resonance comes from the word resonate or to be in tune, in synchronization, in balance. Stress causes a block in the flow of energy, which in turn causes disease and illness.

META-Therapy helps to remove these blocks, allowing the body to heal itself.

META-Therapy is non-invasive, painless and strengthens the immune system. It's even safe for pregnant women and children.

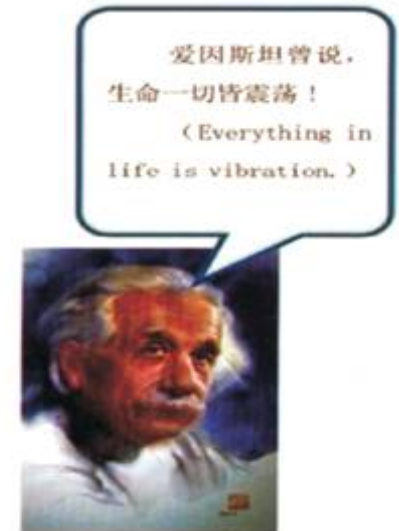

NLS diagnostic and therapy

How Bioresonance Therapy Works

Bioresonance therapy 8Da uses the strategic placement of magnetic inductors on the surface of the head. Electromagnetic signals are transmitted through the headphones in order to clear blockages in the body's natural flow of energy. Several sessions are necessary. Multiple sessions are used as the first couple of sessions are used to create a diagnosis of the degree of blockage associated with the patient's illness. Computer hookups record data as the electrodes administer the treatments.

For many centuries proven natural healing methods, like acupuncture, homeopathy and healing with plants, have used this principle with great success. META-therapy builds upon this foundation, but in a totally new synthesis utilizing modern computer technology and electronics. This makes it possible always to find the right frequencies, which are specifically tailored towards the patient and which are most effective for the treatment. The therapy system transmits this information from the computer to the body in exactly determined amounts and activates self healing and the elimination of toxins.

NLS diagnostic and therapy

The **META-therapy** main feature in the 8D is that activity to adjust automatically, and it's not necessary to strengthen physiological fluctuations separately and to invert the pathological that the device can do it all automatically; you only need click '**Start**', select the necessary section, and therapy runs.

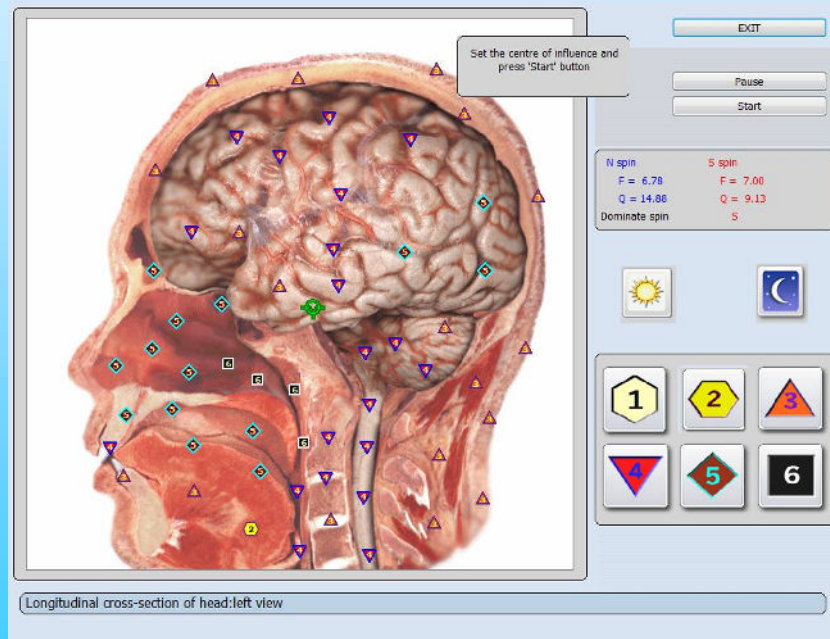


Fig.32.

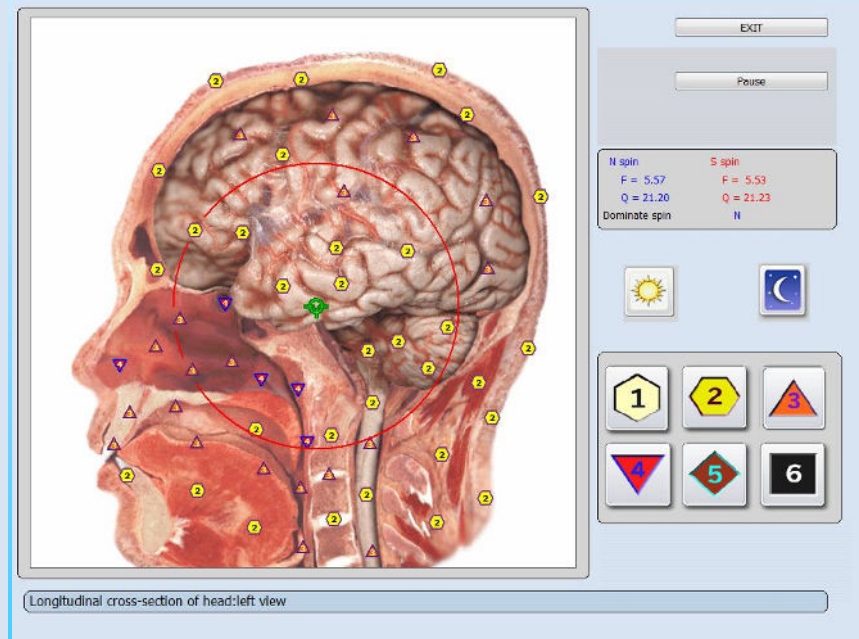


Fig.33.

NLS diagnostic and therapy

The therapy-session consists of two steps:

A: For diagnosis the therapist utilizing the computer system 8D determines problems of your body, causes of stresses and blockages of your energy system.

B: For therapy you receive the exact amount of frequency information for your healing.

All biological processes within a body are governed by the higher energy of the meridians and the central nervous system. Because of our modern way of living these processes can be severely disturbed because of both internal and external stress, excessive demands, unnatural food products, electro smog, environmental toxins, and geopathic stress. The body reacts with chronic permanent stress. This stress can result in a malfunction of the immune system. The results: a full spectrum of different symptoms, exhaustion, allergies, chronic diseases.

In such a situation it is useless to treat individual symptoms. Permanent healing is only possible with a complete detoxification of the body, with stress reduction and a reactivation of the regulatory systems, which means the meridians and the central nervous system. At this point META therapy is very effective.

NLS diagnostic and therapy

The **META-therapy** helps the body to better deal with the discovered problems, toxins and allergens and to eliminate these. In addition the higher causal factors of organic disturbance - chronic stress and disturbed reactions of the central nervous system - will be neutralized due to the therapy. Both are important factors for the activation of the immune system and self healing, enabling the healing of even very old organ diseases.

The course of treatment need 1 sessions every other day. totally need 10 sessions. It is advisable to do not more than 5-6 organs Meta-therapy for 1 session.

A therapy session lasts from about 5---20 minutes. How long the treatment has to be repeated depends on the nature of the illness. Normally 3 ---10 sessions are required.

At preventive care, it is recommended to perform 1 session every other day, totally need 10 sessions.

If want to make Meta-therapy again, suggest to relax for one month. When treat for diseases, 1 session per day, treat 5-6 organs for 1 session, suggest to relax for 2---3 weeks, then you can treat again.

NLS diagnostic and therapy

In addition to the therapy, the practitioner many times prescribes trace elements, homeopathic remedies, herb teas or other supplements. These will be individually tested for effectiveness and form an optimum extension of the therapy.

The therapy between the two magnetic heads of the 8D headphones is pleasant and relaxing. It optimizes the energy system of the body and boosts the immune system and the capacity for self healing. The patients feel more vital, more active and have more energy - often even after the first therapy session. The ability to tolerate stress or external demands of daily life improves. Pain and symptoms often reduce even after the first session.

Despite it's effectiveness **META-therapy** is a very gentle treatment. The applied electromagnetic fields are relatively weak in comparison to our usual exposure of manmade electromagnetic fields. Side effects and risks are not known. Therefore the META-therapy is also ideally suited for children.

NLS diagnostic and therapy

The Causes of stresses


The following causes of problems and stresses in the body can be determined with 8D and can be treated:

Organs: Are there chronic infections, degeneration or metabolic disturbances? Autoimmune deficiencies? Risks of tumors?

Tissues, skeleton, muscles, blood: Are environmental toxins or metabolic toxins stored? What is the individual reaction to these? Are there acute or chronic infections? Stresses?

Central nervous system: Which stress reactions are present due to emotional issues or external excessive demands? Which detox reactions are blocked as a result of these? What effect does it have on the body?

Toxins + Allergens: Are there stresses due to heavy metals (i.e. lead, cadmium)? Stresses due to environmental toxins or pollutants (formaldehyde, solvents, pesticides, etc.)? Are there food allergies (milk, pork, wheat, yeast, additives)? Other allergies: pollen, pets, dust, fungus, etc.? Electromog or geopathic stress?

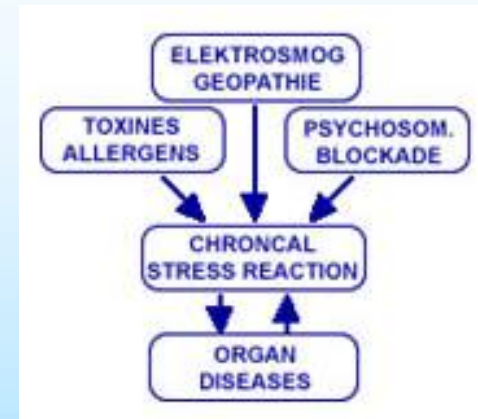

NLS diagnostic and therapy

Healing through information

The acupuncture meridians and all systems of the body which receive information and energy from these meridians, the nerves, the organs and the body tissues, can be positively influenced with the proper information signal. Such signals for example are frequency signals from substances, trace minerals, herbs or homeopathic remedies.

Bioresonance therapy is a painless therapy that deals with the hidden causes of disease and poor health by assessing and then normalizing energetic imbalances. All matter, whether living or inert, resonates at a particular electromagnetic frequency, including the human body. Toxic substances in the body such as infections, chemicals, and heavy metals alter the body's normal pattern and the body begins to adapt to the new frequency, causing illness or other disorders. Using bioresonance to modify and correct energy patterns allows the body to return to its natural healthy state, allowing people to become free of addictions, allergies, and pain.

This is because bioresonance enhances the body's own regulation and detoxification. The body needs to detoxify itself of accumulated waste in order to allow nutrients to be delivered at a cellular level. A healthy diet is necessary along with bioresonance and your therapist will recommend the best diet for you along with any supplements that may be needed.

NLS diagnostic and therapy

8D therapy is aimed at correcting the deranged intro bodily balance and corresponding electromagnetic radiation via information preparations (metazodes).

8D metazodes are specific combinations of frequencies found to resonate with the current state of ill-health (the pathological waveforms are inverted by 180°). They can be received by the client via the 8D itself or transferred to a matrix (Water, Alcohol, Sugar, Paraffin) for oral delivery over a course of treatment. This method of treatment is similar to that used in the NES-Pro treatment protocol and accounts for a wide sphere of influence of this type of preparation and the absence of harmful side effects and contraindications in the cases when conventional remedies are prescribed simultaneously.

The NLS analyze and META-therapy, which were developed in Russia, are the modern methods for the effective holistic analyze and therapy of chronic diseases, pains and general ill health.

For the first time in energy medicine, META-therapy not only treats the organs but in addition also treats energy blocks in the autonomic nervous system and the central nervous system - systematically and routinely.

The self regulation of the body is decisively activated, enhancing the ability of the body to heal itself. The causes of any illness are treated, rather than the symptoms or the individual organs.

The word “META-therapy” was first used by its inventor, the Russian physician Dr. Grig Butov. It stands for the therapy goal of treating the whole person.

META-therapy works with the device “8D”, a new diagnosis and therapy machine of the energy medicine, which links the traditional complementary-medical system and modern results of research in one synthesis. Using META-therapy the biological stimulation is maintainable without medication.

META-therapy is a medical appliance, but it is not able to cure serious diseases on its own. Reducing or stopping medication depends on the results of the therapy which has to be discussed with your medical attendant.

NLS diagnostic and therapy

If you click the button **Meta-therapy** you will enter a mode which allows to carry out bioresonant therapy of an organ. Choose the centre of influence on the picture of the given organ having positioned the mouse cursor on a green circle in its necessary part.



it is "Protector". (System Default)



it is "Destructor". (Not suggest to use)

"**Protector**" and "**Destructor**" buttons are used to change the character of effect.

"Protector" mode wave function of healthy tissue is increased, resulting in activation of compensatory reaction of tissue.

"Destructor" mode wave function of pathological agent is suppressed, resulting in decreasing of adaptive reactions level.

NLS diagnostic and therapy

META-Therapy with 8D has achieved excellent results in the following areas:

1. chronic - degenerative illnesses of all kinds, autoimmune diseases, adjunct therapy to tumors.
2. weak immune system, chronic infections.
3. acute and chronic pain and inflammation.
4. fatigue, exhaustion, sleep disorders, depressions, migraine, psychosomatic illnesses.
5. allergies, chemical sensitivity, electro sensitivity, eczema, neurodermatitis, environmental medicine.
6. hormonal disturbances, menopausal difficulties, PMS.
7. old age illnesses.
8. pediatrics: growth problems, behavioral difficulties.
9. spinal symptoms: back pains, pains in joints, tensions, arthritis.
10. injuries, bone fractures.
11. sports medicine, preparation for competition.

Notice: Like all other medical therapies, META-Therapy is not always able to be successful for all patients and in all cases. If a META treatment does not yield the desired effect further medical diagnosis and treatment might be necessary.

NLS diagnostic and therapy

Comparative analysis , (If you after making the Meta-therapy, you can do this comparative analysis, it will show you the different)

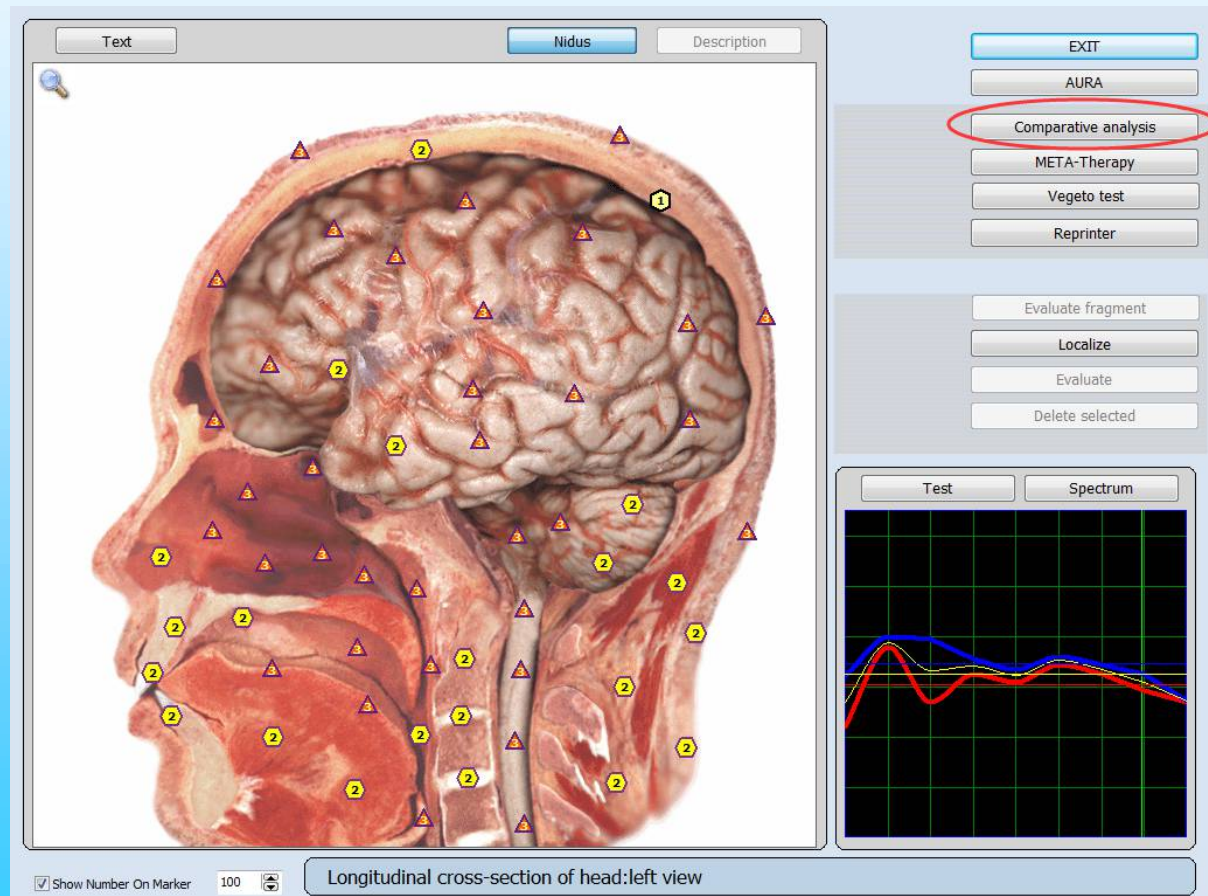


Fig.34.

NLS diagnostic and therapy

Put a tick opposite the investigated organ and its picture will appear at the bottom window on the left. Then simply click this organ with a mouse after Meta-therapy and in the right window there will be the same organ after investigation (Fig.35)
(in detail you can find it in the chapters: Current analysis – Comparative analysis).

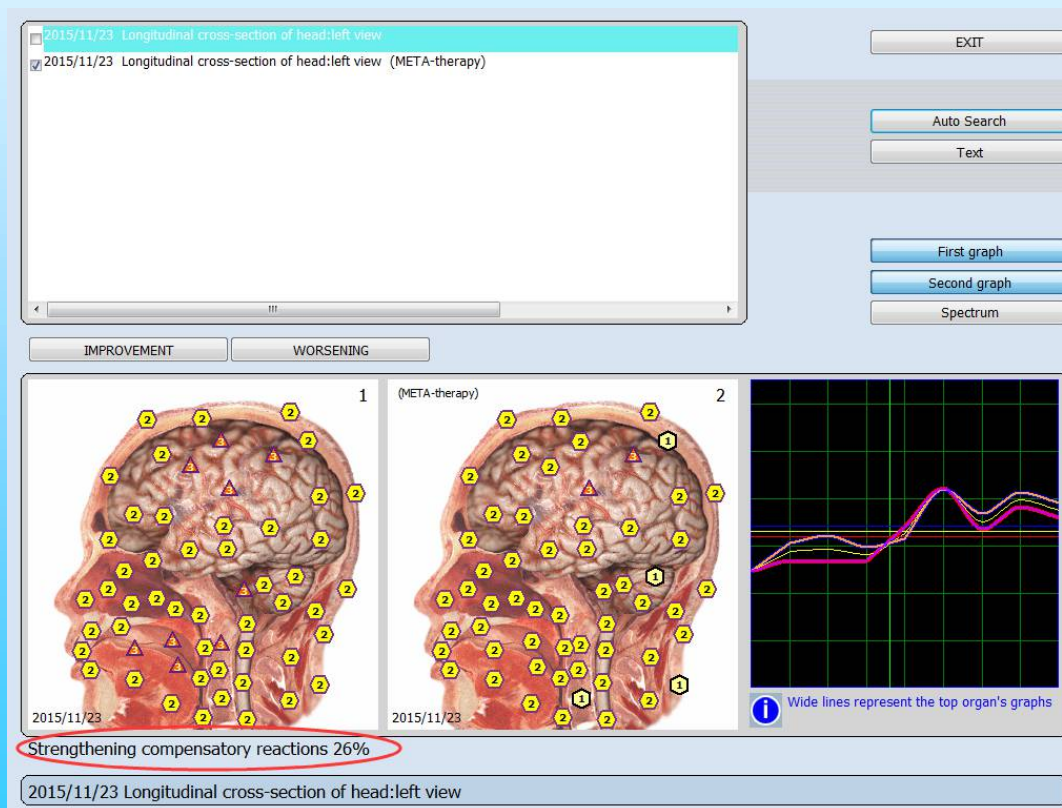


Fig.35.

NLS diagnostic and therapy

The comparative analysis (Fig. 35) allows to estimate the results of influence on the organ. At the top of the screen the list of all fulfilled researches is located. Choose with a tick the research which you want to compare. It will appear in the picture on the left. Then choose another research of the same organ. In the center of the screen there will be an inscription about the increase or reduction of compensatory reactions of the organ in the second research.

Sorting of researches in the given window is identical to sorting of researches in a window of the Card file. You can return to a card file and sort researches by date or alphabetically, and then return to the given window. **Auto search** allows to find automatically the results of research of the same organ which is chosen with a tick. In the centre you can see the result of the comparative analysis.

(Everytime you make the comparative analysis, should click the Auto search,it will show you different)

NLS diagnostic and therapy

When you click the **Auto search** (Fig.36), In the bottom of the screen the program will show the increase (in the given case on 26%) or reduction of compensatory reactions of the organ after the influence of the given etalon on it.

To close this page and return to the page of standards it is necessary to click **Exit** and on the opened page click the key **Test**, located at the left over the graph.

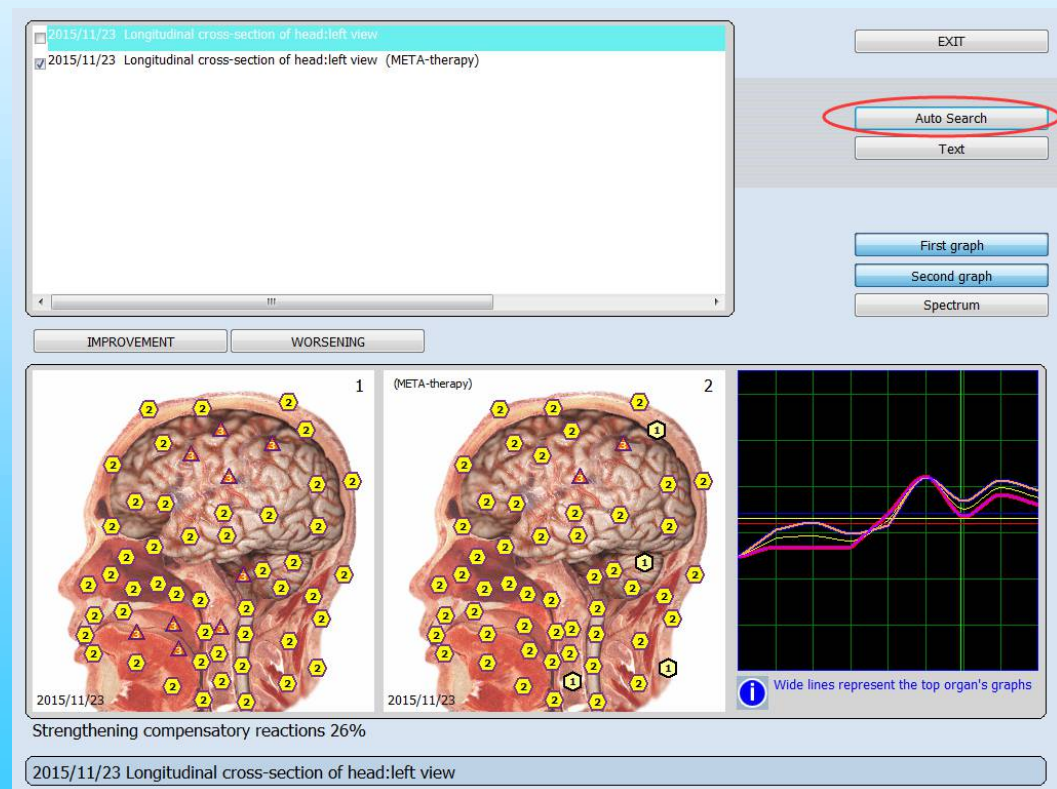


Fig.36.

NLS diagnostic and therapy

For example: strengthening of compensatory reactions to 9 %. It means the general improvement in the second case in comparison with the first. You can observe the influence in details be looked by pressing **Improvement** and **Worsening** to the right of the pictures.

When you click the **Improvement** the points with parametres very close to the standard will start to blink on the pictures of an organ.

After pressing **Worsening** the points which have significant deviation from the standard will blink.

Thus influence of this medicine has weakened compensatory reactions of the organ in these parts. It is necessary to carry out additional examination for selection of other standard which will compensate weakening. (We know that drastic antibacterial medicines weaken digestive and immune systems. Therefore compensatory medicines, probiotics and prebiotics are prescribed together with them). Also it is possible to compare the results of influence with the help of curves of the processes.

Test : shows green crosses on pictures of organs with the corresponding description of parts of organs. At the bottom part of the screen you can see the name of the chosen organ.

Exit : To finish your work with the comparative analysis menu.

NLS diagnostic and therapy

Vegeto test (external)

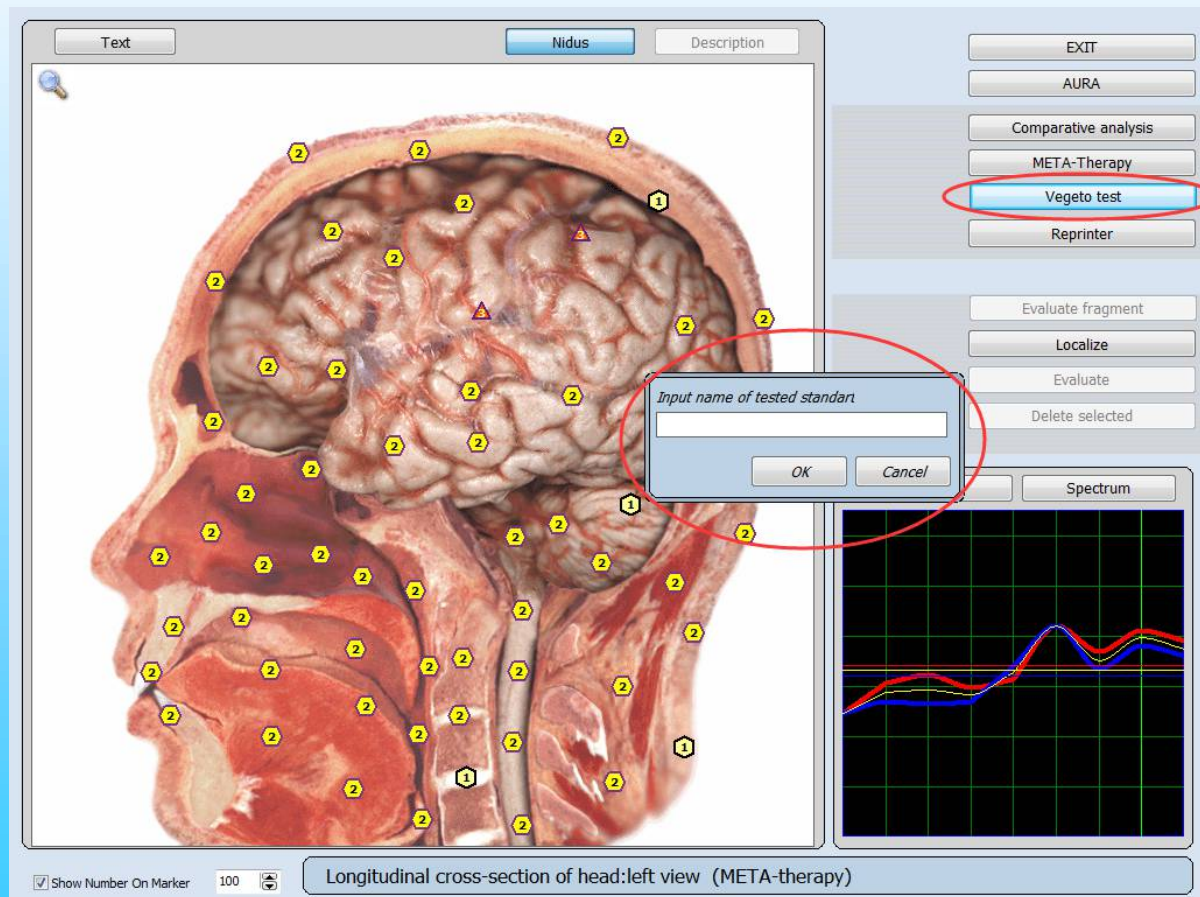


Fig.37.

NLS diagnostic and therapy

The given button allows to carry out external Vegeto test with the use of the resonant chamber to check the efficiency of standards which were not included into the matrix. The device database contains a considerable quantity of etalons and the device can simulate the results of their application and possible negative consequences. To check the efficiency of medicine which is not in the catalogue of the program put it into the resonant chamber and click the **Vegeto test**. Then, you will be suggested to put down the name of the etalon into the entry line of the open window. Next, click **OK**, and testing will begin automatically. Please click **Cancel** if you wish to leave the menu(Fig.37).

Further use the comparative analysis to evaluate efficiency of the given medicine for this organ. Compare the virtual model of the organ during research to the virtual model of the organ after the use of etalon, and evaluate strengthening/weakening compensatory reactions of the organism.

If you wish to test the etalon from the catalogue of the program, first enter the window **Test** and then in this window choose **Vegeto test**.

NLS diagnostic and therapy

One of the more popular uses of the 8D is the “Vegeto test” . The control of the vegetative resonance brings understandable ideas and news of the manner in which various medicines can affect the human body. We know that the material world possesses frequencies just as the human body. These frequencies contain an information and this information can be read by the 8D.

The frequencies of a medication can get into harmony with a person or not. This idea is transformed into the principle of resonance. The closer the frequency of the medication is to our frequency, the more efficient it is. That is why it is important to choose alimentary additives, homeopathic formula, allopathic remedies, vitamins and plants (phyto-aroma) according to the principle of resonance.

The Vegeto control of 8D can be used to verify the adjustment of a medication to the problem organ of a person. There are two ways to proceed. Either by comparison of a pre-existing medicine found in the given database, or by verifying the relevance of a medication the patient already uses.

NLS diagnostic and therapy

In the first case, we have to choose a medication presenting a low spectral similitude. The lower it is, the better it is (f.inst. 0540 or 0350). Click on the '**Vegeto test**' button, and treat the organ with the chosen medication. Then with the help of the function '**Comparative analysis**' it is possible to see the change in the organ and whether the patient ought to take this medicine. The organ will either improve or degenerate. Thus it only remains to choose the medicine which is already in use or the most efficient new one suggested by 8D.

In the second case, we want to check a medicine the patient already is using. In this case, we have to use the container and the laser to test the frequencies of the resonance of this medication. Click on the button 'Vegeto test' and write in the name of the medicament to be tested. Then proceed to sweep the organ in question. The effect can be analysed in the same manner as the medicaments in the database.

Many therapists use the 8D technology exclusively to determine the ideal medication for their clients and to evaluate the effect.

Click the 'Test'

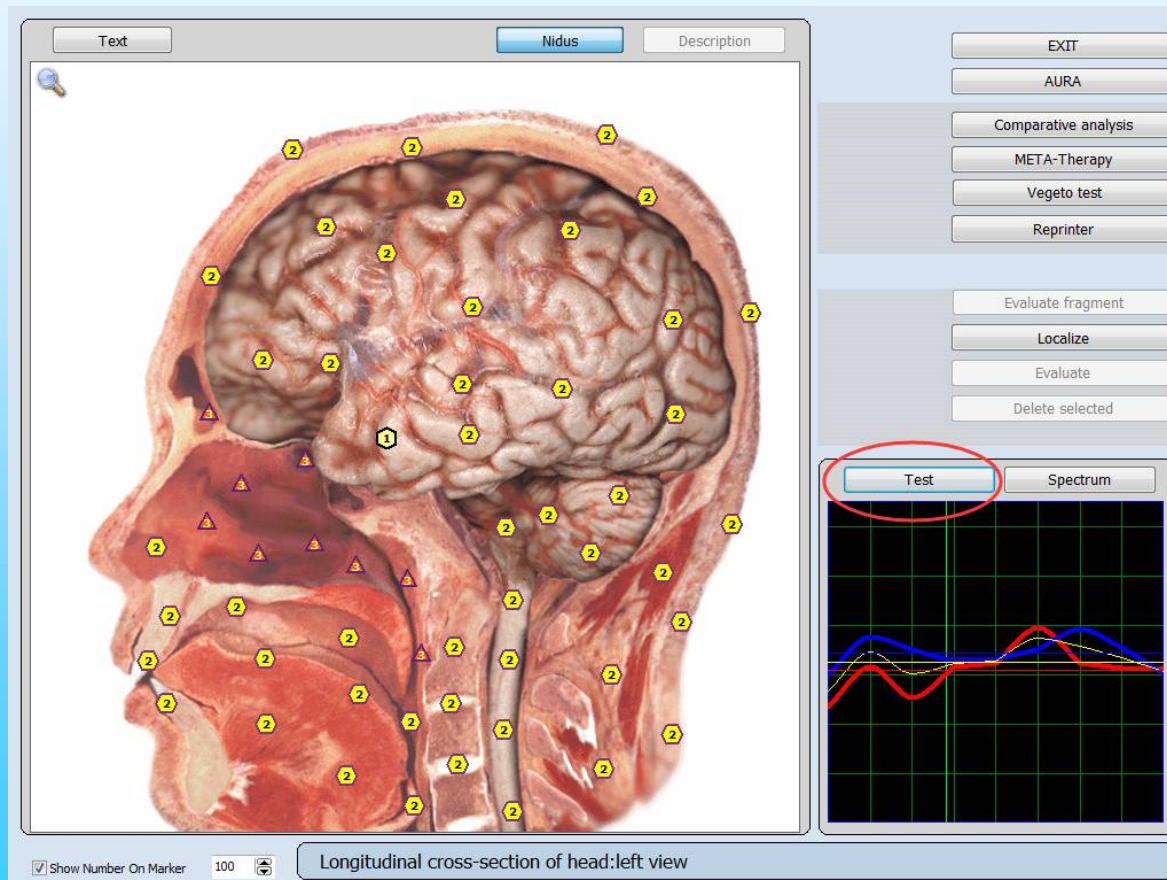


Fig.38.

NLS diagnostic and therapy

Let's start with the button the Test, located on the left over the graphes of processes. You get to a window of Etalon(Fig.39). On the left you can see groups of etalons - a table of contents. In the central window—etalons of this group.

Opposite each etalon there is a figure which corresponds to similarity of a spectrum of the investigated organ to the etalon. The smaller the figure, the closer the curves are. If the figure is less than 0.425 similarity is great enough and these etalons are marked with red colour. If the figure is in an interval 0.425 – 0.750 – similarity to the etalon is not essential. If the figure is more than 0.750 similarity to the etalon is not identified.

The figure also means the time of disease happening between this time and the next time. (The greater the value the farther away from that is the lower the chance that). Generally speaking 0.425 is basic parameters of disease occurring. Such as the number is less than 0.425 showing the disease is occurring.

For example, By Entropy analysis in the 5-7 grade and the number is less than 0.425, the disease is currently taking place.

NLS diagnostic and therapy

It will appear this page (Etalon list)

The screenshot displays the NLS diagnostic and therapy software interface. The top section features a list of topics for selection, including Nutraceuticals and parapharmaceuticals, Organic preparations, Biochemical homeostasis, Pathomorphology and nosological, Microorganisms and helminths, Allopathy, Homeopathy, Phytotherapy, Lithotherapy, and Food. A spectral graph is shown with two lines (blue and orange) plotted on a grid. The x-axis ranges from 1.8 to 8.2, and the y-axis ranges from 1 to 6. The graph shows a blue line with peaks at approximately 2.6, 4.2, and 5.8, and an orange line with peaks at approximately 2.6 and 4.2. The bottom section displays the Etalon list according to decreasing spectral similarity, with a table showing three entries: Cross section of abdomen at the level of 1st lumbar vertebra, Optimum distribution, and Virtual model. The interface includes various buttons for navigation and analysis, such as Spectrum, Object, Etalon, Model, Invert, Optimum, EXIT, Reprinter, Vegeto-test, Auto scan, Etalon description, Etalon-Object, Entropy analysis, NLS-Analysis, To print, View report, Adjustment, Adjust all, Auto model, and Absolute model.

Clear Topic

☐ A # Nutraceuticals and parapharmaceuticals

☐ B # Organic preparations

☐ C # Biochemical homeostasis

☐ D # Pathomorphology and nosological

☐ E # Microorganisms and helminths

☐ F # Allopathy

☐ G # Homeopathy

☐ H # Phytotherapy

☐ I # Lithotherapy

☐ J # Food

Spectrum

Object

Etalon

Model

Invert

Optimum

EXIT

Reprinter

Vegeto-test

Auto scan

Etalon description

Etalon-Object

Entropy analysis

NLS-Analysis

To print

View report

Adjustment

Adjust all

Auto model

Absolute model

Fix Sort Select Show all Smart filter

0	0.000	Cross section of abdomen at the level of 1st lumbar vertebra
0	3.527	Optimum distribution
☒ 0		Virtual model

Search

Cross section of abdomen at the level of 1st lumbar vertebra

Fig.39.

NLS diagnostic and therapy

There are the following control elements:

Clear : which is above the list of etalons shuts off the opportunity of dispersion analysis simultaneously for all groups of etalons.

Topic : setup show or hidden groups of etalons.

Fix : allows fixing these three lines in the top part of the list:
Biological object name.
Optimal distribution.
Virtual model.

Sort : automatically sorts all etalons alphabetically.

Select : automatically sorts all etalons by similarity of their names from different manufacturers of etalons. The line of search in lower left corner, under the list of etalons enables to find the required etalon very quickly by introducing some of the first letters in its name.

To view other buttons of this window let's take the Herbal medicine (phytotherapy) as an example.

Smart Filter : allows selecting a group of etalons similar to each other by the last word in their name.

NLS diagnostic and therapy

Spectrum : pressing this button displays an enlarged graph.

Object : graph lines of lilac and orange color, display a graph of the examined biological object, organ or tissue plotted in the course of the investigation.

Etalon : thin graph lines of red and blue colors, represent a graph of the chosen reference process.

Model : thick graph lines of red and blue colors, show a graph of the virtual model.

Invert : enables the polarity of the graph to be inverted.

Optimum : a yellow graph shows normal (Gaussian) distribution of the signal in standard frequency.

NLS diagnostic and therapy

Auto scan: allows to carry out Entropy analysis and Biochemical analysis automatically. If you click this key again the analysis will stop. (Usually not suggest to use this button)

Etalon-Object: To estimate what etalons are connected with the etalon you are interested in.

Entropy Analysis: Show two factors, which shows a mathematical model of pathological process taking place within healthy tissue. (It will introduce later.)

NLS Analysis: Carry out a multifactor entropy analysis of the pathological process (biochemical homeostasis of the system). (It will introduce later.)

To print: Indicate in the printout etalons with a high spectral similarity to the object under investigation. This sends the item highlighted into the memory of the printing page.

View report: Show you the report page prior to printing.

Adjustment: Virtual activation of a pathological process, even if in remission it may be of interest to us. Pressing this button causes tuning of the chosen reference process to the spectral characteristics of the object under investigation and shows the process in its activation phase, within the 4th row.

Adjust all: When clicked causes the tuning of ALL reference processes stored in the etalons directory referred to under Adjustment. This is the button necessary to do prior to view and interpretation (Entropy Analysis) of current disease states.

Absolute model: A quick way to identify areas of concern

NLS diagnostic and therapy

Etalon testing

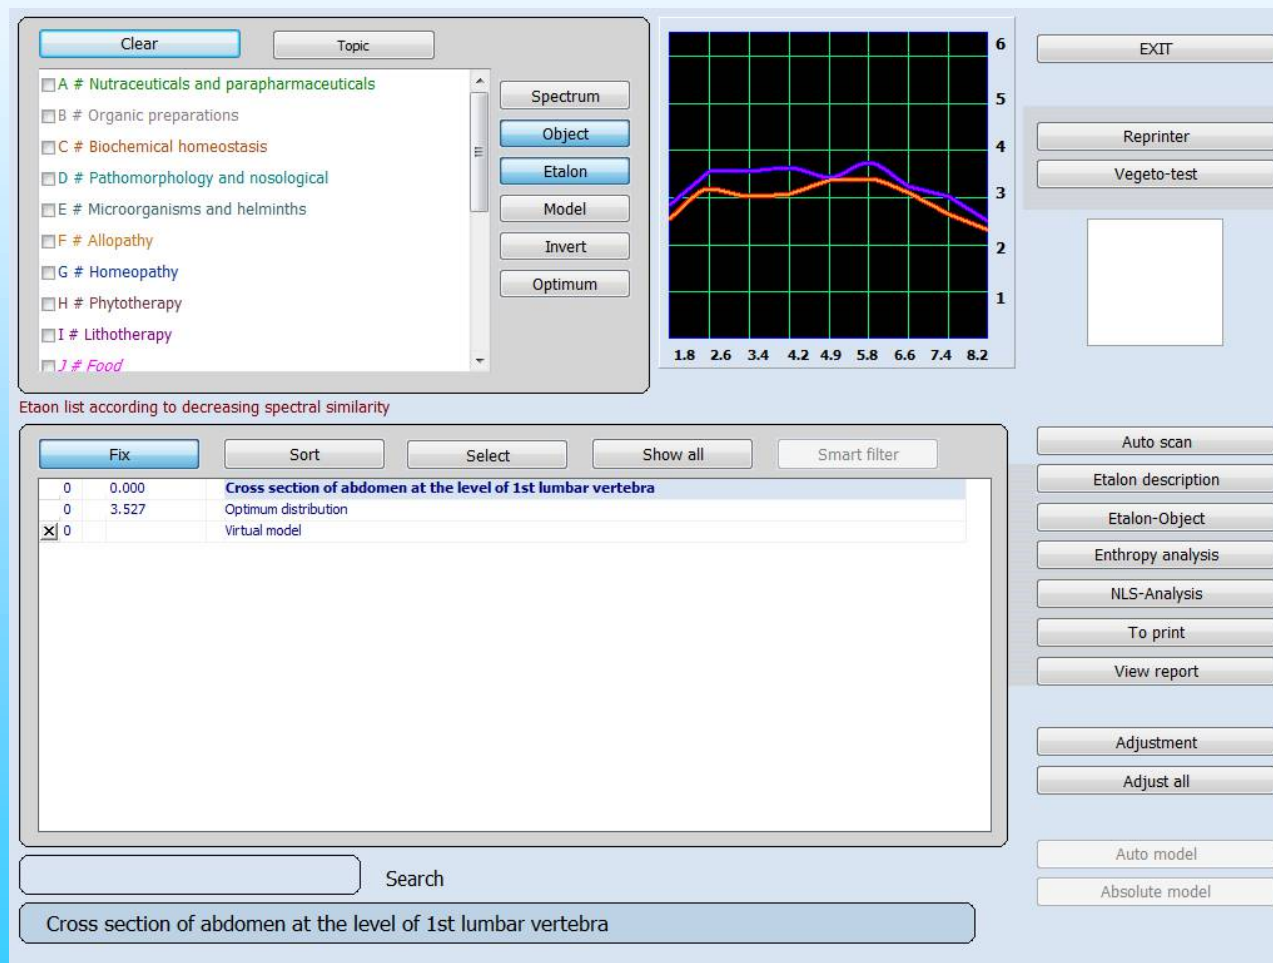


Fig.40.

NLS diagnostic and therapy

Every organ and every cell has its own specific and distinctive oscillation. The oscillations are stored in the computer memory and can be displayed on the screen as a graph, which represents the condition of the information exchange between an organ or tissue and the environment. Every pathology has its own individual and distinctive graph. The computer memory also stores a very large number of pathological processes taking into account rate of evidence, age, sex and other variations. After frequency characteristics are read from tissue, the apparatus compares spectral similarity with stored processes (healthy tissue, pathological tissue, infection agents) and then selects the closest pathological process or tendencies to its appearance.

By this method of analysis it is possible to trace the condition of the red (S) input signal and the condition of the blue (N) output signal, which are displayed as graphs on the screen. From the shape of the graph it is possible to determine which of the reference (etalon) processes it appears to be closest to and to check the spectral similarity of the graph plotted for the patient.

Curves of pathology

In the analysis of entropy there are curves which indicate the degree of entropy (from 1 to 7) at different frequencies (1, 6 to 8,2 Hz) both for structure (blue curve) and for function (red curve). By a healthy state, the two curves follow each other closely all the way. A large discrepancy between the two curves indicate a pathological process within the communication system of the body.

NLS diagnostic and therapy

Natural frequencies of the tissues within the following standard frequency band(Fig.39.8):

- 1.8 skeletal system;
- 2.6 coarse connective tissue, joints, and cardiac valves;
- 2.6 - 3.4 loose connective tissue, striated muscular, and cardiac muscle;
- 3.4 unstriated muscular tissue.
- 4.2 tessellated epithelium of the digestive tract;
- 4.9 stratified squamous and columnar epithelia. Parenchymatous liver tissue and tissue of the biliary tract;
- 4.9 - 5.8 kidney tissue epithelium and reproductive organs;
- 5.8 lymphoid ring of the pharynx, upper section of the respiratory tract, lymphatic system, spleen, ovaries, and prostate;
- 6.6 peripheral nervous system, bronchus epithelium, adrenals, and thyroid;
- 7.4 central sections of sensory analysers except the optic ones, and sub cortical structures of the brain, pons cerebelli; cerebellum, limbic system and lungs parenchyma;
- 8.2 retina, optic nerve, cerebral cortex.

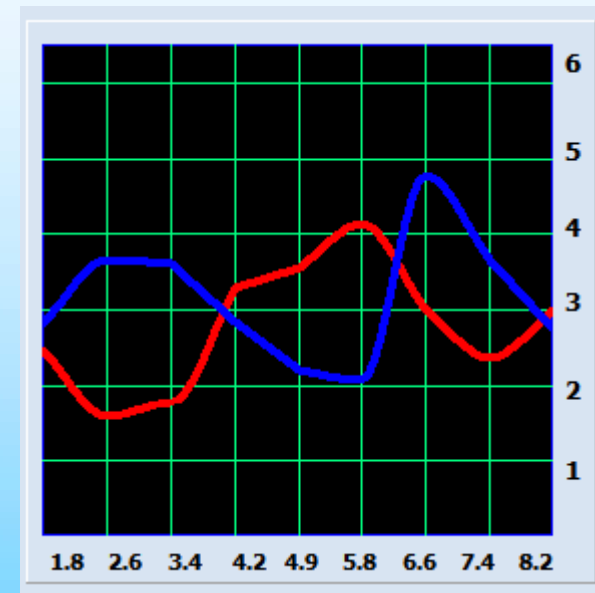


Fig.41.

NLS diagnostic and therapy

Basis of "8D" apparatus' works is measuring of the noise rate in a system. We consider any system (organ, tissue, cell, etc.) as cybernetic system ("White box"). Comparing input signal (red, S) and output signal (blue, N) we can evaluate system's condition and dynamic of entropy increasing - entropic potential.

In ideal system input and output signals are similar - it means that there's no noise in the system. And vice versa, if system does not respond to control signal - we can say that the system is not functioning.

In practice we work with intermediate values, evaluating which we can say about acuteness, priority and dynamics of process development. To make it more convenient we use graph amplitude scale in which 0 dB means 0 points and 260 dB means 6.6 points. Any tissue has a natural noise rate at about 8.5 - 64 dB, that means 1 - 3 points. We consider graph amplitude within (Fig.39.2) - 6.5 points, numbers exceeding the bounds means that the system is not functional. Self resonance frequencies have a great importance in graphs analysis. The higher organized tissue is - the higher it's maximum frequency, for example, bones have maximum amplitude 1.8 Hz, and brain cortex - 8.2 Hz. Mind that we do not consider S and N graphs separately. In that case they do not have a sense. We consider them together, focusing on frequencies that have more dissociation and on the graph that placed higher. Isolines can simplify process of analysis. Analyzing their position and point rate we can reveal acute-ness and dynamics of the process, it will help greatly in further treatment.

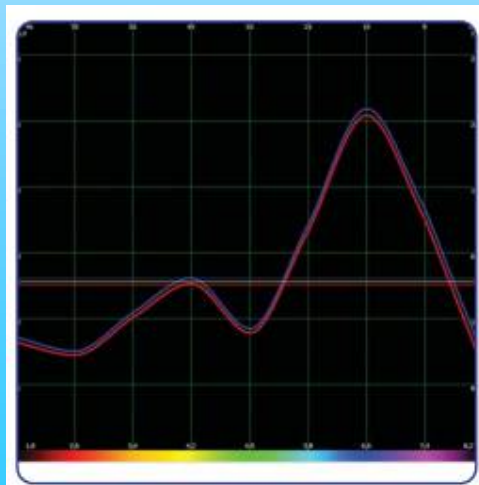


Fig.42.

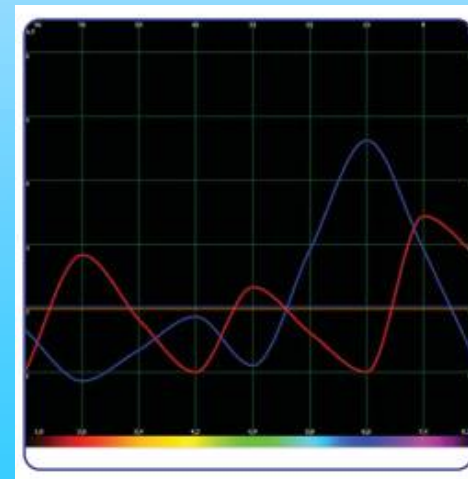


Fig.43.

NLS diagnostic and therapy

Using "Spectrum" function we can see graph of the process it three isolines: yellow one is the simple average of both graphs, blue and red ones are isolines of input and output signals.

To analyze the process we use several factors. To estimate compensatory reactions we analyze interval between N and S isolines. The process is compensated if interval is less than 0.25 points, in other case the process is decompensated.

The most productive is compensated process: it can be regulated, self reserve of the system can resist pathological process without assistance, at the same time reserves of tissue and organism work synchronously. There are two type of decompensated processes: anabolic and catabolic.

Anabolic process characterized by positive prognosis of clinical course and goes with energy and information discharge. In that case blue isoline is higher than red one. Decompensated anabolic process characterizes quick acute processes (phlegmon, abscess, and pneumonia, often with autoimmune allergy component) with decreasing of adaptive functions of organism and high hyperergic tissue reactions. Suppressing of the disease goes at tissue level.

Reserves of compensations of single tissue quickly run out and process course becomes crisis one. If there are enough reserves, process comes to compensated stage, in other case - into catabolic process, it means loss of control by organ or tissue.

At catabolic process red line placed higher than blue one. This process' course is characterized by absorption of information and energy. At initial stage of catabolic process it can be unpronounced, it characterizes chronic diseases and in the same time middle isoline has 3.5 points and higher. With further development of catabolic process middle isoline goes up to 5.5 points and graph voltage is decreasing (voltage means interval between peaks of graph and it's isoline).

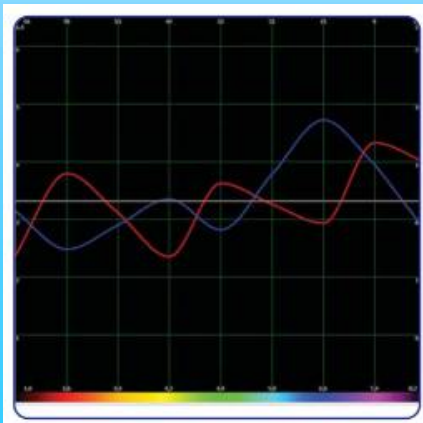


Fig.44.

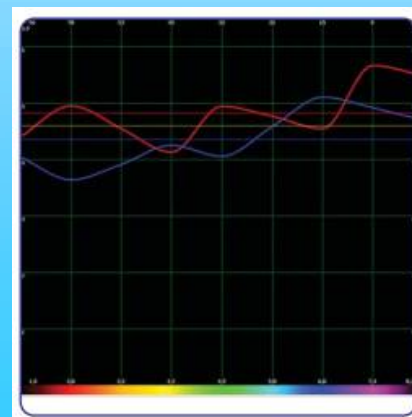


Fig.45.

NLS diagnostic and therapy

The tissue cannot react to input signal - interval between red and blue isolines increasing, organism spends a lot of energy to support tissue's reserves and at the same time reaction of the tissue decreasing. That kind of development is typical for tumors. Non-cancerous tumor are characterized by a small interval between isolines (1 - 1.5 points), cancerous tumors are characterized by interval 3.5 - 4 points. At initial tumor graph has minor voltage on self frequency, at metastatic - graphs are flat. To define the acuteness of the process it is necessary to analyze dissociation of graphs and position of average isoline. At initial acute process significant dissociation can be traced at one frequency and average isoline cannot be higher than 2.5 points. The secondary acute process average isoline goes up to 3.5 - 4 points and higher, dissociation of graphs on more than one frequency.

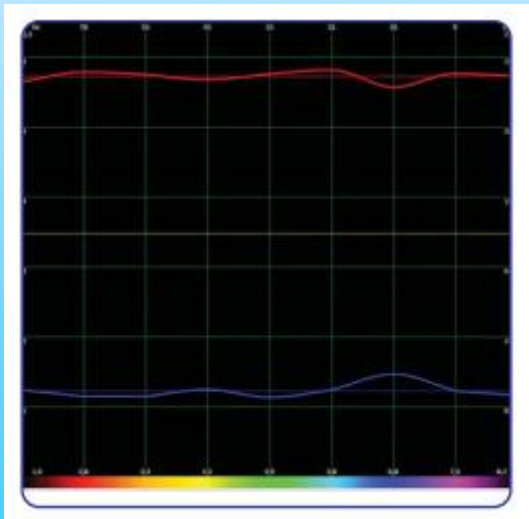


Fig.46.

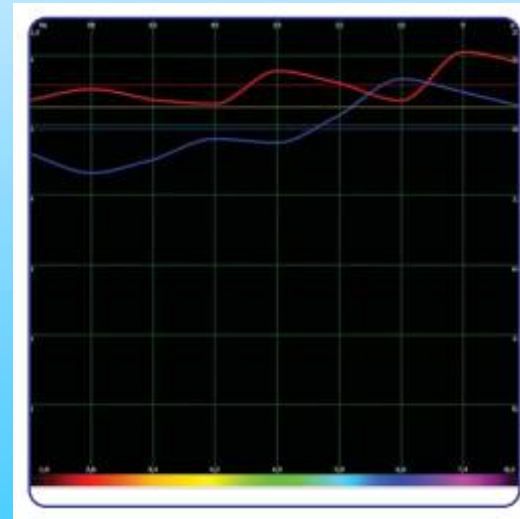


Fig.47.

NLS diagnostic and therapy

"Group List" contains a list of common etalon groups:

NUTRACEUTICALS AND PARAPHARMACEUTICALS

In this group the wave characteristics of biologically active supplements (BAS) produced by major Russian and foreign companies who produce and supply nutritional supplements are recorded.

ORGANIC PREPARATIONS

Contains the etalons (standards) of the spectral characteristics of healthy body tissues.

The etalon list is arranged in a decreasing order of spectral similarity to the object under investigation. Healthy tissue has similar input and output signals (the red and blue graphs respectively).

The greater the similarity between the organ preparation and the object under investigation, the more intact the tissue will be. Conversely, the greater the difference the greater the damage will be to the tissue under investigation.

NLS diagnostic and therapy

BIOCHEMICAL HOMEOSTASIS

This program carries out a qualitative evaluation of the main biochemical factors by evaluating the wave functions of body tissues. This evaluation is carried out using the NLS - analysis mode.

Note that the lowest values of enzyme (hormone) concentration within the normal bounds correspond to 2 in the graph.

Whereas, the highest values within the normal bounds correspond to 6. The values of the factors equal to 3, 4 or 5 correspond to the 'mode' of the factor, and the extreme values 1 and 7 characterize biochemical factors beyond the physiological norms, lower and higher respectively.

The standard rules for making biochemical analysis using conventional clinical methods should be used when analyzing the computer results.

PATHOMORPHOLOGY AND NOSOLOGICAL

This shows a list of the etalons of destructive processes.

This section holds basic patomorphologic conditions peculiar to single tissues of an organism. Every destructive process has a distinctive graph.

NLS diagnostic and therapy

MICROORGANISMS AND HELMINTHS

In this section are recorded the major characteristics of infection agents: bacteria, viruses, mycoplasma, rickettsias, fungi and helminths. This presents changes in the form of high peaks of dissociation within the frequency range representing the natural frequencies of the tissue.

For example *Opisthorchis felineus* has a high dissociation in frequency - 4.9Hz - parenchymatous liver tissue and bile excreting tissue. These tissues are known to be largely affected by trematodes *Opisthorchis felineus* opisthorchiasis.

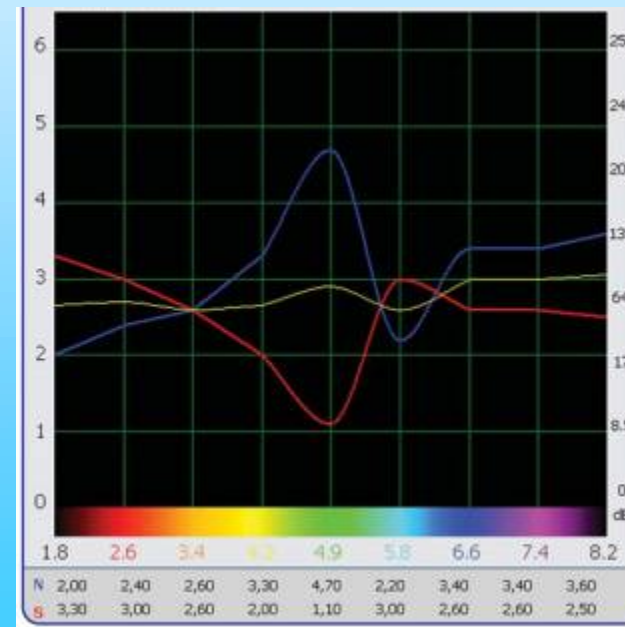


Fig.48.

NLS diagnostic and therapy

ALLOPATHY

In this group the wave characteristics of the principal chemical (synthetic) medicinal preparations used in conventional medicine.

HOMEOPATHY

In this group the wave characteristics of homeopathic preparations are recorded.

PHYTOTHERAPY

In this group the wave characteristics of medicinal plants growing in the Midwest of Russia are recorded

NLS diagnostic and therapy

If put a tick on the left in the menu **Phytotherapy**.

In the central window you will see Etalons for Phytotherapy.

Three etalons have appeared in the red zone (their index number is less than 0.425).

It means that the wave functions of this etalon combined with the wave function of the organ approach this etalon as much as possible and that is healthy(Fig.49)

Vegeto-test (internal)

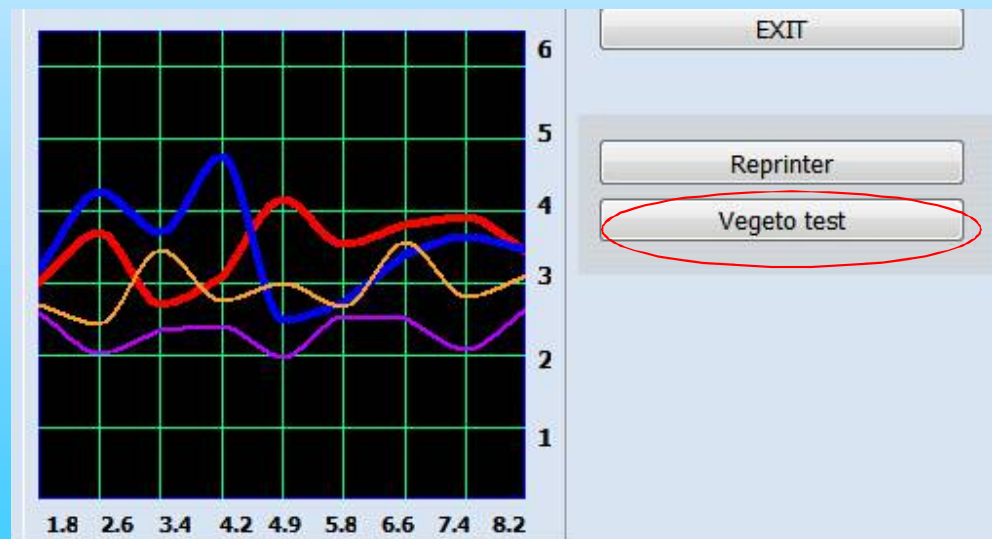


Fig.50.

0.349	PETROSELINUM SATIVUM HOFFM*
0.410	CALTHA PALUSTRIS*
0.411	ADONIS VERNALIS*

Fig.49.

The program allows to simulate the process of influence of a chosen etalon to an organ. For this purpose we choose an etalon and carry out the **Vegeto test** (headphones should be on a head of the client). Choose the etalon and click a button Vegeto-test situated on the right (Fig.50), the Vegeto-test will begin automatically.

NLS diagnostic and therapy

FOOD

In this group wave characteristics of food separated into groups (meat, fish,dairy, vegetables, fruits, oil, drinks, spices,etc.) are recorded. Dietetic foodstuff, due to their therapeutic action recommended to use, highlighted in red color. Not recommended foodstuff highlighted in black, neutral - in pink

ALLERGENS

In this group wave characteristics of food, domestic, animal, vegetable, and industrial allergens of all kinds are recorded.

LITHOTHERAPY

In the program spectral characteristics of gems and minerals are represented together with description of therapeutic action. By pressing "Picture" button you can see pictures of minerals. Program can choose a mineral for a patient,suitable according to spectral characteristics for permanent possession or for specific diseases treatment. Using specific spectral characteristics of minerals, modulated and radiated by the apparatus, you can treat acute and chronic diseases.

NLS diagnostic and therapy

BACH FLOWERS

**S7 SAHARARA corresponding meridians: VC +
VGcorrespondingcorrespondingmeridiansmeridians: VC + VG: V**

**S6 AJNA corresponding meridians: MC +
TRcorrespondingcorrespondingmeridiansmeridians: MC + TR: MC +**

**S5 VISHUDHA corresponding meridians: P + GI + Sk +
Sdcorrespondingcorrespondingmeridiansmeridians: P**

**S4 ANAHATA corresponding meridians: C +
IGcorrespondingcorrespondingmeridiansmeridians: C + IG: C +**

**S3 MANIPURA corresponding meridians: F + VB + Fd +
Adcorrespondingcorrespondingmeridiansmeridians: F**

**S2 SVADHISTANA corresponding meridians: R + V + ALL +
Lycorrespondingcorrespondingmeridiansmeridians**

**S1 MULADHARA corresponding meridians: RP +
Ecorrespondingcorrespondingmeridiansmeridians: RP + E: RP**

NLS diagnostic and therapy

ENTROPY ANALYSIS.

Click ' **D# PATHOMORPHOLOGY AND NOSOLOGICAL** ' and **Entropy Analysis**

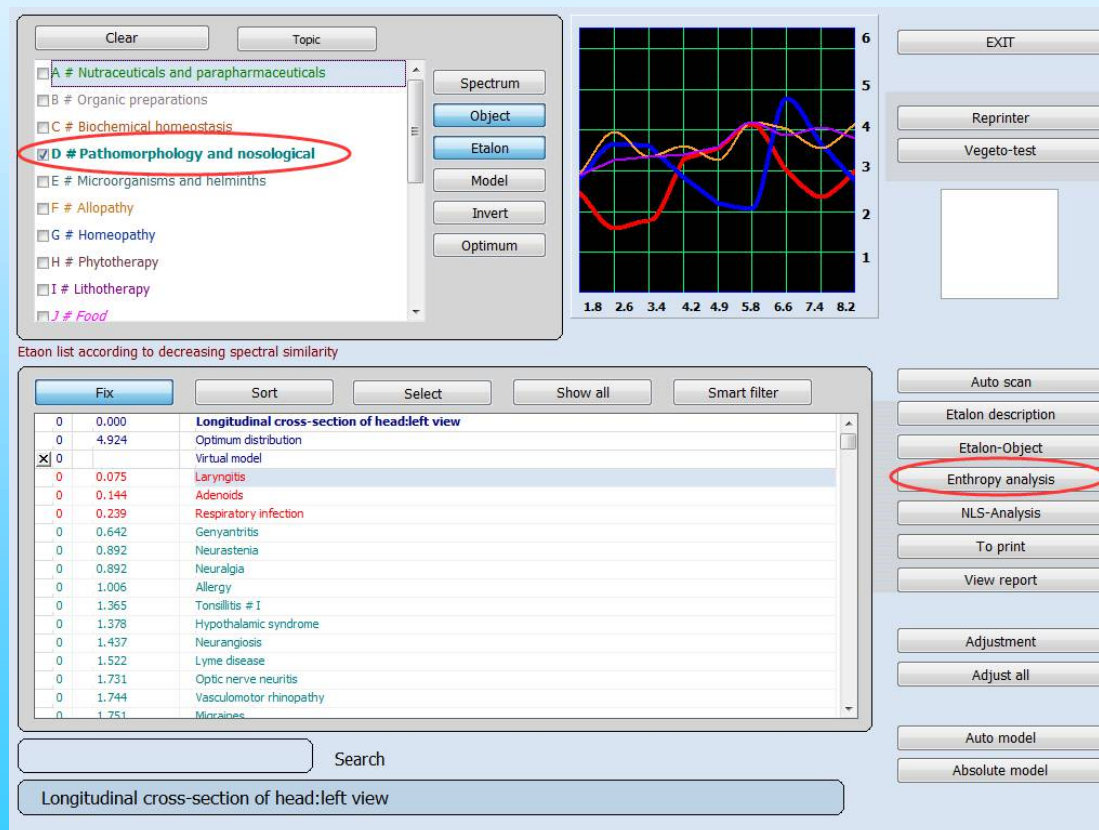


Fig.51.

NLS diagnostic and therapy

It will show this page.

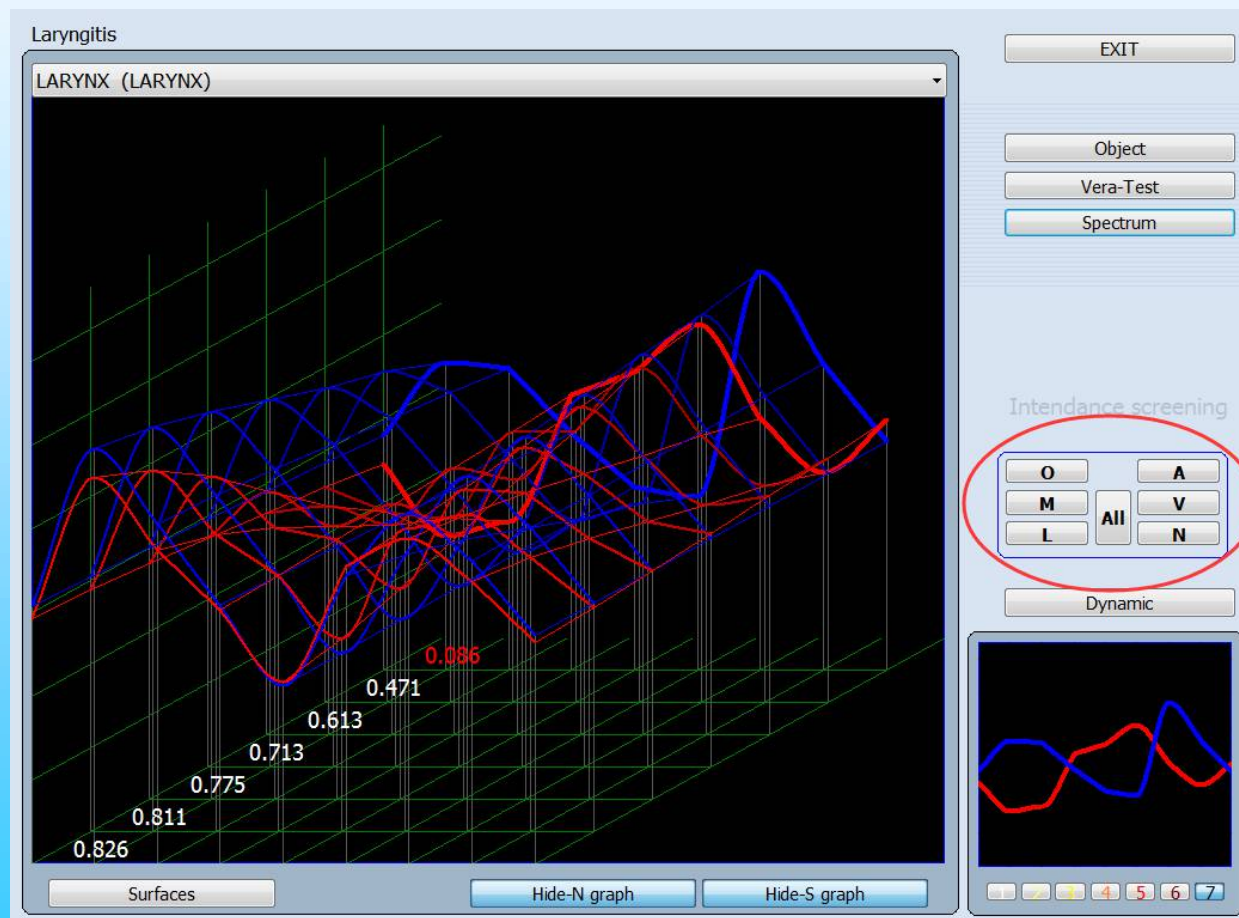


Fig.52.

NLS diagnostic and therapy

Entropy (two-factor) analysis enables to build a mathematical mode of pathological process taking healthy tissue (organopreparation) as the initial (zero) phase and a clinically pronounced form of a pathological process as the final one and making a mathematical calculation for the graphs of a number of intermediate states. In the course of analysis the highest spectral similarity to any of the intermediate states or extreme states gets determined and thus maturity of this process and signs of a preclinical pathology are defined.

A small difference in the spectral similarity (dispersion) over the whole range of entropy factors from cates an acute process. The most similar graph in terms of the spectrum is marked by a thick line in the graph and the digital value red, is marked red, in this case it is 0.536. There are two buttons '**Conceal N(S) graph**' that the button hides the corresponding graph(Fig.52).

One can also view the graph in the mode '**Surfaces**' by pressing the button 'Surfaces', to get back to the mode '**Lines**' it is necessary to release this button.

NLS diagnostic and therapy

ENTROPY ANALYSIS of the relationship between the human brain, consciousness and physiological phenomena physical analysis, that is Varying degrees of damage from the disease in the body of the six systems :

Muscl (**Muscular system**)
Lymph (**Lymphatic system**)



Artery (**Arterial system**)
Vein (**Venous system**)
Nerve (**Nervous system**)



The rest of the groups tissues not included in the above mentioned list.

The button **Object** displays the optimum values for this process.

The button **Vera-Test** represents a graph with the closest spectral similarity.

One by one to analyze and calculate the disease in the human brain, the left mark, Such as the average value **All** we can get a comprehensive analysis of the integrated value of their symptoms within six systems. If the higher the value, the physiological illnesses phenomenon more retained in the brain consciousness, the greater their physiological responses and human feeling is more obvious.

NLS diagnostic and therapy

Click '**All**', then click the '**Exit**', it will show you this number.

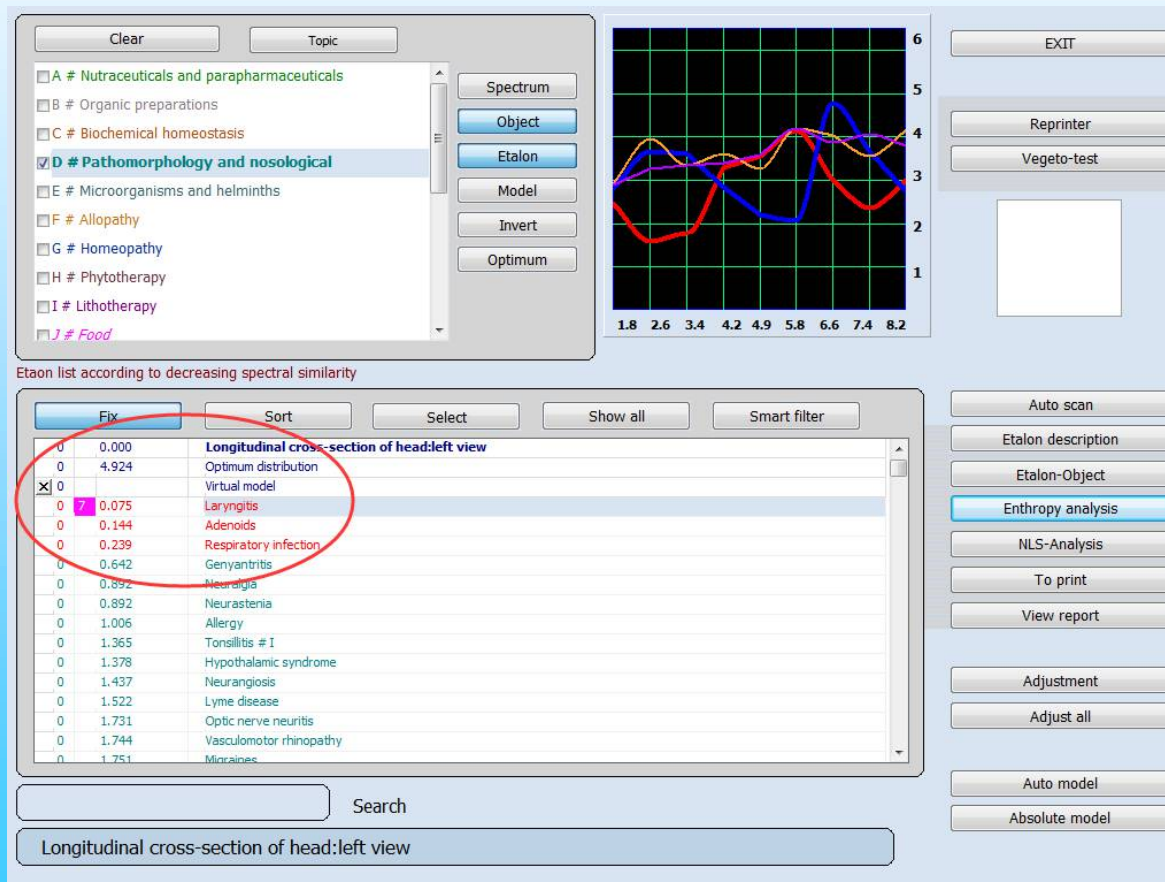


Fig.53.


NLS diagnostic and therapy

Entropy analysis

In a window of etalons there is a button of Entropy analysis (the button is active only for etalons of pathomorphology) which opens the given window (Fig.54)

The Entropy analysis allows to make 2 factor analysis of the etalon. Thus the program builds mathematical model of pathological process, taking as an initial stage a healthy tissue and for a final clinically expressed form of the given pathology.

In this window we first of all are guided by degree of maturity of process (from 1 to 7), which is indicated in the bottom part of the small graph. Thus entropy maturity indicator can be:

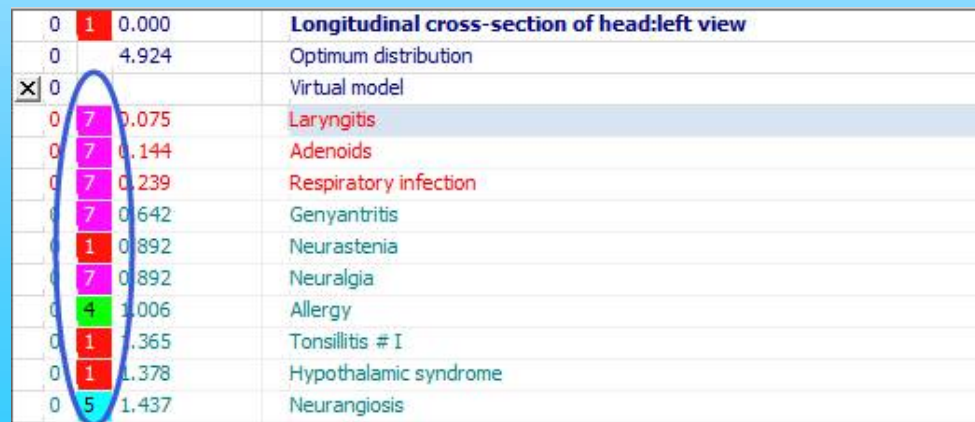

0	1	0.000	Longitudinal cross-section of head:left view
0		4.924	Optimum distribution
0			Virtual model
0	7	0.075	Laryngitis
0	7	0.144	Adenoids
0	7	0.239	Respiratory infection
0	7	0.642	Genyantritis
0	1	0.892	Neurastenia
0	7	0.892	Neuralgia
0	4	1.006	Allergy
0	1	1.365	Tonsillitis # I
0	1	1.378	Hypothalamic syndrome
0	5	1.437	Neurangiosis

Fig.54.

NLS diagnostic and therapy

E value (In the third column):

1--2 - indicate that there is no tendencies in the development process under investigation (means the disease on the body external response is not obvious).

3--4 - indicate that there are preclinical phases in the development process (means the disease on the body external reaction occasionally, or it will reflect by external causes).

5--7 - indicate that in the maturity process (means the disease reaction is more obvious or often happen on the body external).

Thus, the higher the figure, the more mature the process is, and the diagnosis is especially definite.

Then the same figure will be highlighted next to the diagnosis in the list of etalons when we return back to the previous page.

NLS diagnostic and therapy

Then click the **'Adjustment'** and **'Adjust all'**.

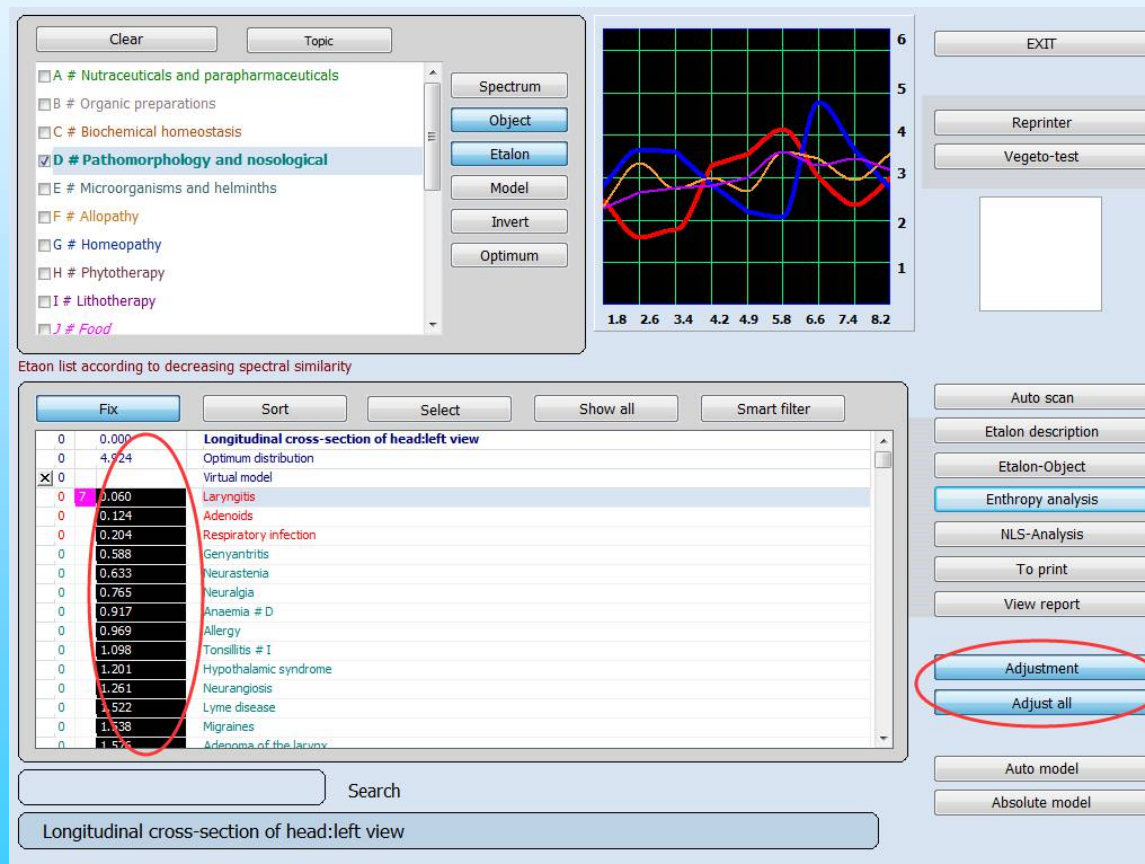


Fig.55.

NLS diagnostic and therapy

Adjustment and Adjust all.

As it has been already mentioned there is a zone from 0.425 to 0.75 where similarity of etalon and organ spectra is insignificant. Etalons which are recommended for compensation are situated in this zone:

- the chronic diseases which are in condition of remission (out of an aggravation),
- diseases to which the organ is predisposed.

To define more precisely we use **Adjust all** (as though it were a virtual provocation) of the organ. The computer simulates the reaction of an organism in case of stress. If after simulation the etalon factor becomes less than 0.425 (has passed to the red zone), it means that there is a functional disorder and it is necessary take appropriate measures.

As with any adverse influence this process can pass from predisposition or remission to an acute phase. If the factor has not changed much, the organ has enough reserves and the given etalon is not expedient.

Here it is important to understand that the organism during the given particular period of time cannot deal with all problems at once, therefore those etalons which are useful to an organism at present are usually highlighted in a red zone (without provocation).

NLS diagnostic and therapy

If you click the button **Adjust all**, the computer will simulate the changes of a condition of an organ in stress and will pick up compensating standards itself (Fig.56)

0	0.374	PETROSELINUM SATIVUM HOFFM*
0	0.380	ADONIS VERNALIS*
0	0.418	LINUM*
0	0.429	HUMULUS*

Fig.56.

In this example **LINUM** has appeared in the a red zone (compare Fig 44 and Fig 46). The index has considerably decreased and even has turned to the red zone, therefore it is useful to choose it as one of the recommended etalons.

If you are interested in any particular etalon for preventive maintenance and treatment processes out of an aggravation zone point this etalon with the cursor and click the button **Adjustment**. The program will estimate efficiency of this etalon specifically.

NLS diagnostic and therapy

D value (In the fourth column)

If >2.0 , Means lack of any matching samples, the morbidity is very small.

If $2.0 \sim 0.425$, It may not have symptoms now, but still need to attention, if you don't do any change, this problem maybe will happen soon (chronic).

If <0.425 , Red index, the morbidity is higher about 85% ~ 95%.

0	0.000	Longitudinal cross-section of head:left view
0	4.924	Optimum distribution
x 0		Virtual model
0	7 0.060	Laryngitis
0	0.124	Adenoids
0	0.204	Respiratory infection
0	0.588	Genyantritis
0	0.633	Neurastenia
0	0.765	Neuralgia
0	0.917	Anaemia # D
0	0.969	Allergy
0	1.008	Tonsillitis # I

Fig.57

NLS diagnostic and therapy

Auto model and Absolute model

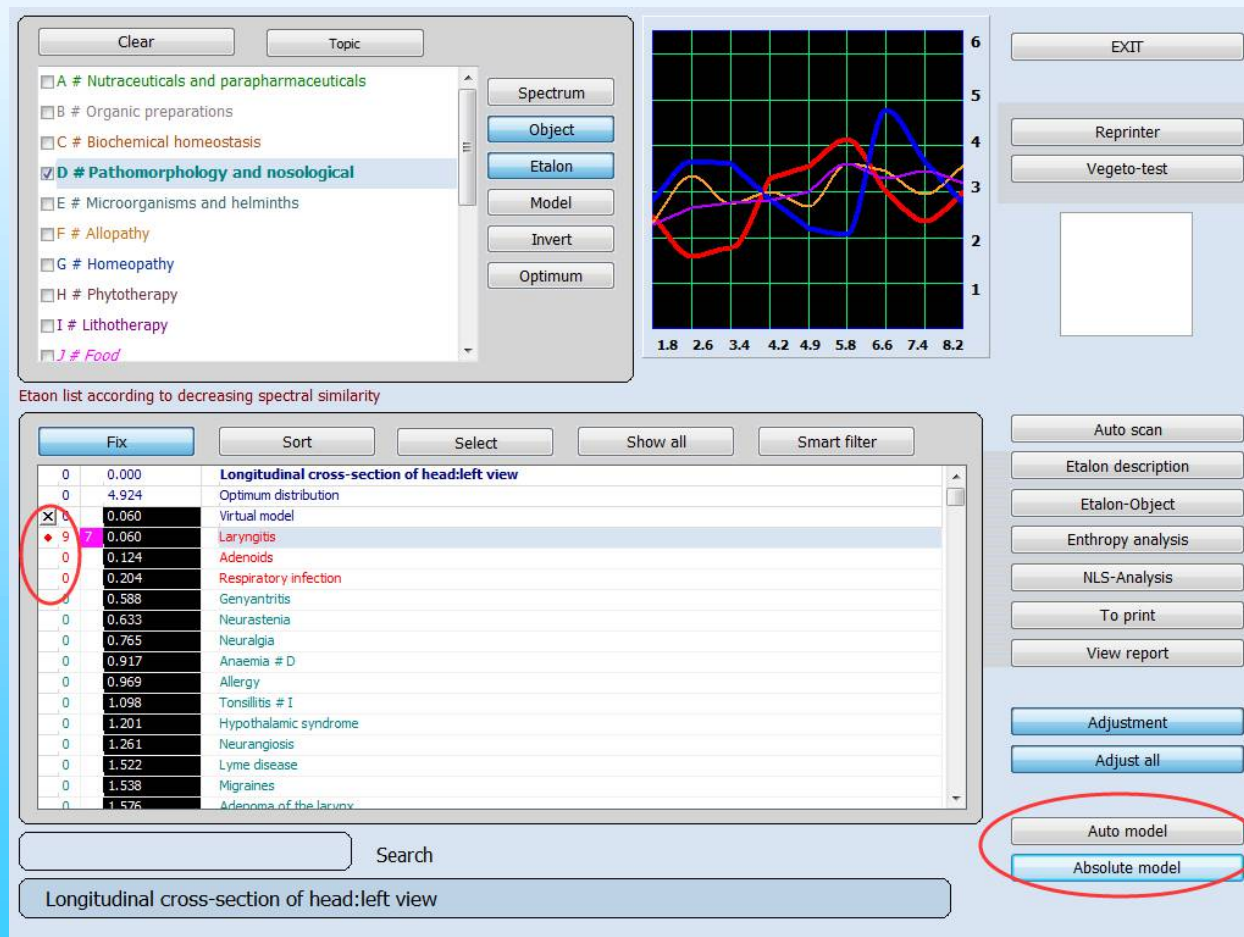


Fig.58.

NLS diagnostic and therapy

Absolute and Auto model

To select an ideal combination of etalons the Absolute model and Imperative model is used (Fig.44).

Absolute model allows to pick up in an automatic mode such quantitative and qualitative combination of etalons that the sum of the cords for the etalons and the organ corresponded to etalon organ. The number that appears to the left of the etalon defines the contribution to compensating curve.

Then it is possible to make one more Vegeto-test and to check the influence of the given qualitative and quantitative selection of etalons to compensatory body's reactions.

If there is a desire to pick up combination independently it is necessary to click the left button of the mouse to the left of the etalons. Red points and figures will be there. The figure defines a share of the contribution of the given etalon. To delete the etalon from the general list press the right button of the mouse. To clear the list completely press X.

If you strongly wish to recommend any particular etalon to the client choose it and click the button **Auto model**. The program will pick up other standards so that in the sum the curve of the organ, this etalon, and other etalons has approached to the etalon organ as much as possible. This is recommended to be made only in case of of an etalon recommended by the program or if the given etalon is used for preventive maintenance (see below).

NLS diagnostic and therapy

ETAON TEST ACCORDING TO DECREASING SPECTRAL SIMILARITY

			Fix	Sort	Select	Smart filter
•	3	0.349	PETROSELINUM SATIVUM HOFFM*			
	0	0.410	CALTHA PALUSTRIS*			
	0	0.411	ADONIS VERNALIS*			
•	3	0.461	FOENICULUM*			
	0	0.470	RUMEX CONFERTUS*			
	0	0.476	ARCHANGELICA OFFICINALIS*			
	0	0.478	HUMULUS*			

Fig.59.

The meaning of red dot: (Orange arrow)

1. Dots in the first column. It represents the disease have occurred in this state in the life and also have potential warning. If the red dot in the top or upper indicates the disease is developing in this state. For example, **PETROSELINUM SATIVUM HOFFM** which shown on the form.If the red dot appears in the down of the form (such as **blue circle**) and with large number, It means the disease happened before.

2. Numbers in the second column. (Green arrow)

Total are divided into (0, 1, 2, 3, 4, 5, 6, 7, 8, 9, ∞).It indicates the time of the disease happening.

The first level (0—3):Time is short or have occurred in the recent.

The second level (4—6):Time is in the past six months or time of occurrence for too long.

The third level (7—9):Time is one year or more than one year.

The fourth level (∞):Have happened for a long time or long-term.

NLS diagnostic and therapy

NLS-Analysis

Click the 'C# BIOCHEMICAL HOMEOSTASIS' and NLS-Anlysis

Clear Topic

☐ A # Nutraceuticals and parapharmaceuticals

☐ B # Organic preparations

☒ C # Biochemical homeostasis

☐ D # Pathomorphology and nosological

☐ E # Microorganisms and helminths

☐ F # Allopathy

☐ G # Homeopathy

☐ H # Phytotherapy

☐ I # Lithotherapy

☐ J # Food

Spectrum

Object

Etalon

Model

Invert

Optimum

EXIT

Reprinter

Vegeto-test

Auto scan

Etalon description

Etalon-Object

Entropy analysis

NLS-Analysis

To print

View report

Adjustment

Adjust all

Auto model

Absolute model

Etaon list according to decreasing spectral similarity

Fix	Sort	Select	Show all	Smart filter
0	0.000			
0	4.924			
X	0			
0	0.733			
0	0.759			
0	0.893			
0	1.047			
0	1.161			
0	1.327			
0	1.331			
0	1.384			
0	1.399			
0	1.522			
0	1.560			
0	1.579			
0	1.589			
0	1.593			

Longitudinal cross-section of head:left view

Search


Longitudinal cross-section of head:left view

Fig.60.

NLS diagnostic and therapy

NLS-Analysis

BLOOD ERYTHROCYTES more than 5.6 mln in 1 ml
BLOOD ERYTHROCYTES less than 3.3 mln in 1 ml

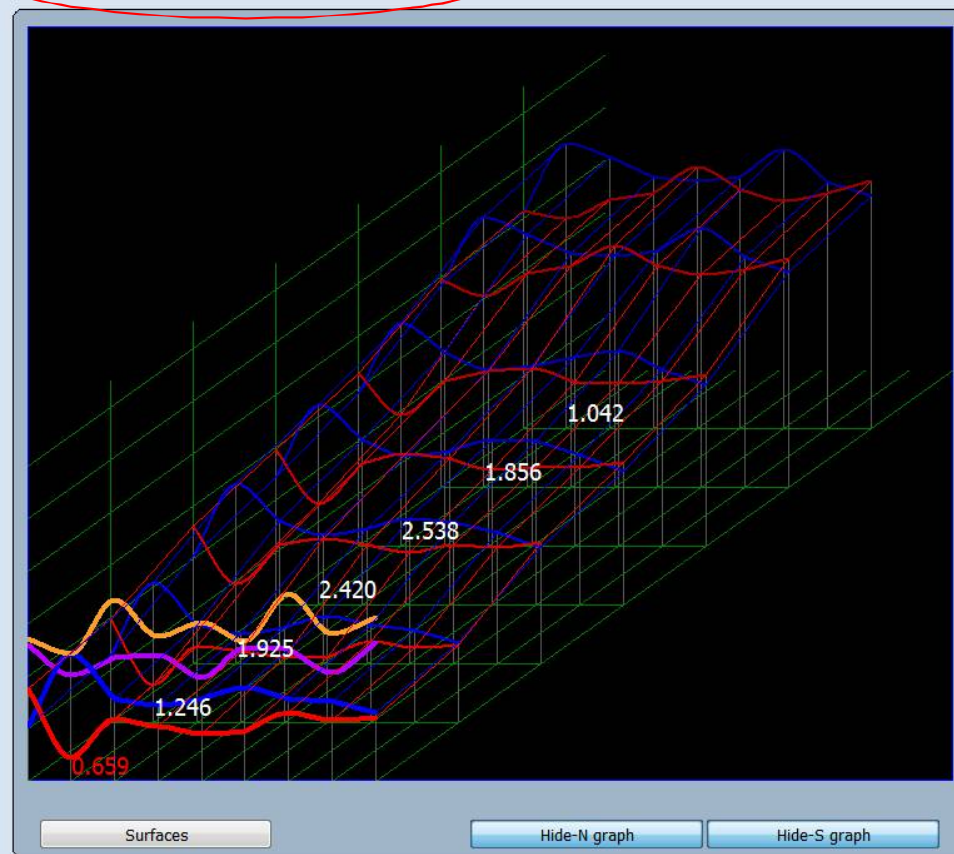

EXIT

Object

Vera-Test

Spectrum

Dynamic




Fig.61.

NLS diagnostic and therapy

Multidimensional NLS-analysis is identical to entropy analysis except that in NLS analysis all intermediate stages are recorded as etalons from patient's bodies in different stages of the developing process under investigation which enables to build a more accurate model of the pathology development. This is a very complicated and laborious type of process record so NLS-analysis is used solely to evaluate malignant processes and biochemical factors.

Analysis of oncoprocesses by an NLS-analysis graph makes it possible to trace the possibility of an irreversible state in the pathology development. Growing amplitude of the output signal (the blue line in the graph) indicates intensification of the compensatory mechanisms. On reaching the maximum value the input signal graph may drop abruptly with high amplitude values of the input signal (red line) which indicates a failure in adaptation mechanisms and development of irreversible states.

NLS diagnostic and therapy

It will show this results.

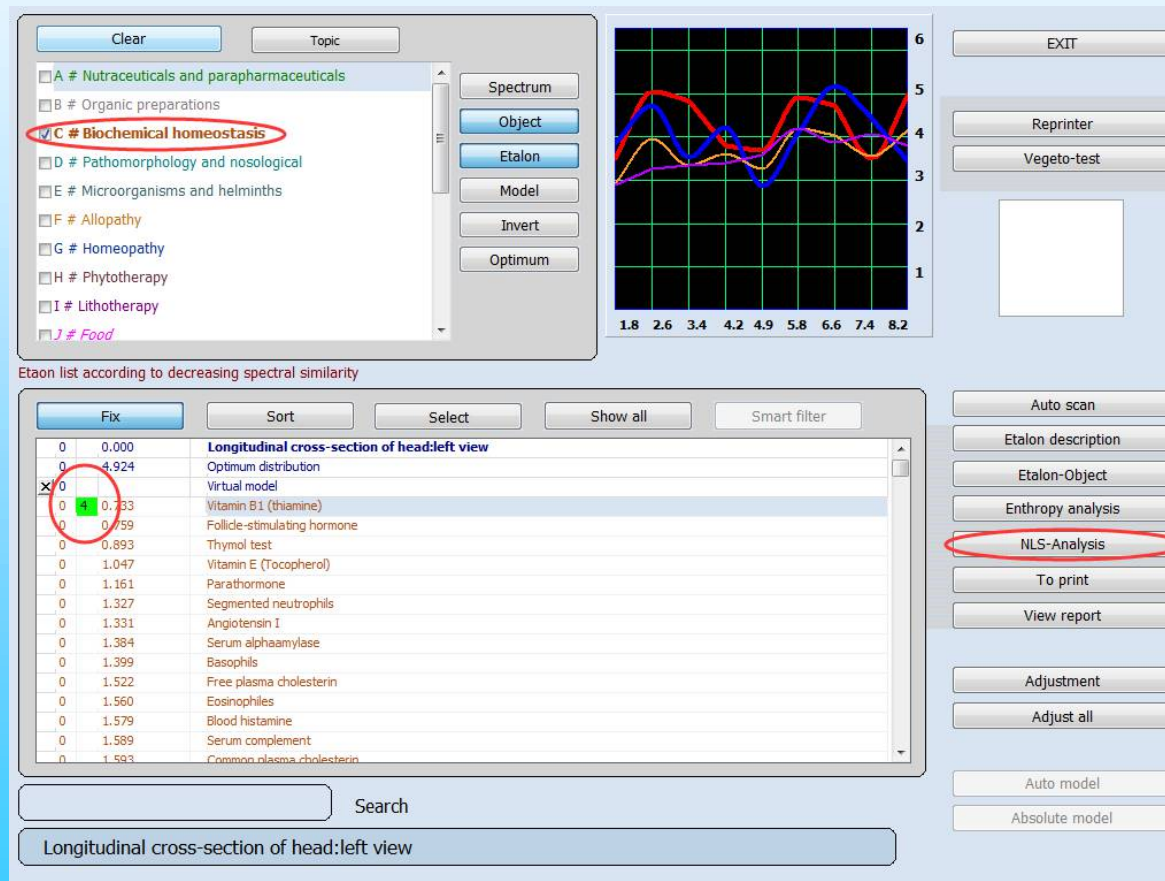


Fig.62.

NLS diagnostic and therapy

The button **NLS-Analysis** is only work for **BIOCHEMICAL HOMEOSTASIS**

The meaning of the **NLS-Analysis** E value:

1, indicates the biochemical index is lower than the standard value range.

2-6, indicates the biochemical index in a safe range.

7, indicates the biochemical index is higher than the standard value range.

If NLS-analysis value is **1** or **7**, you are adviced to go to the hospital for further examination.

NLS diagnostic and therapy

Now the principle of working with the list of etalons is clear:

If we work with Allergens, the substances most dangerous to the given patient causing an allergy appear in the red zone.

If Allopathy is worked, the most suitable medicine to correct the given pathology is in the red zone.

Organotherapy contains etalons for healthy organs and tissues. The closer the indicators of the investigated organ are to the etalon of a healthy organ, the higher the probability of safety both organic and physiological condition of the given organ is. It is necessary to notice that there is no ideal organ so insignificant deviations from the etalon are normal and should be surveyed in details additionally.

If you choose Patomorfolgy the etalons which correspond to various patomorphological conditions or processes will open.

NLS diagnostic and therapy

Allocate the standard you want to check with the cursor and having clicked the left key of the mouse press **Etalon-Object** and the etalon index equal to 0,000 then is given to the etalon, then the etalons subsequent to it (the first two are especially important) are listed according to the degree of importance. In other words it is possible to replace the chosen etalon with the combination of etalons with the same characteristics. If it is an etalon of pathomorphology, the etalons are listed according to the degree of importance in disease process.

By clicking the key **Etalon description** you open a detailed description of the etalon (if it is included in the base).(Fig.63).


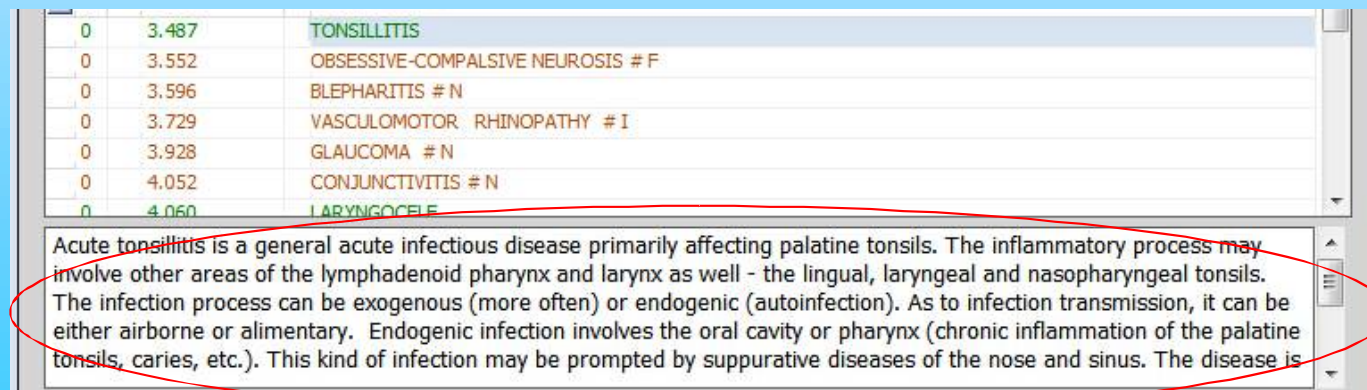


Fig.63.

NLS diagnostic and therapy

To Print : allows to print the chosen etalon processes. The result of the print is a recommendation of operator (exclusively) given to the patient. Therefore, to add each new etalon from the list into print it is necessary to choose this etalon manually.

View report : allows to look though the chosen list of etalons prepared for print and click the button Report, you can print the report.

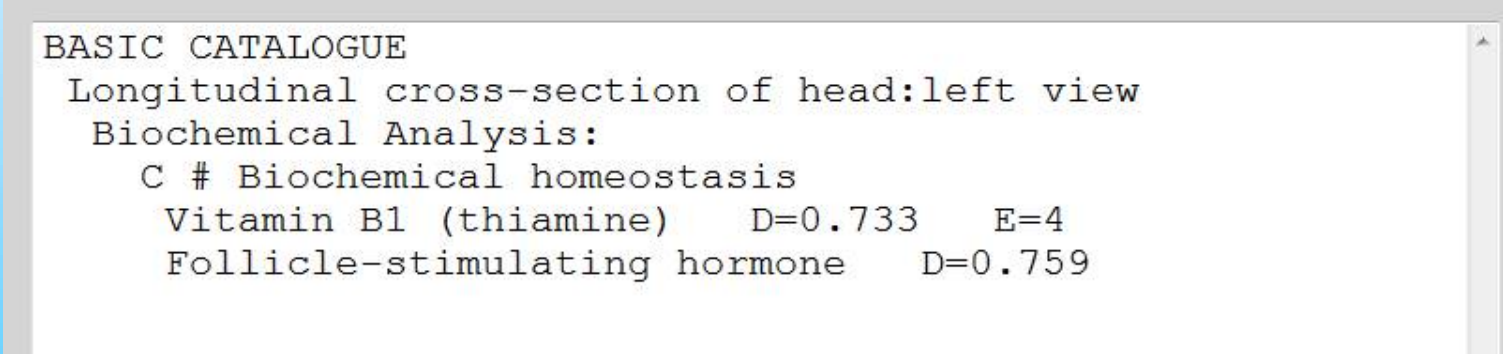

```
BASIC CATALOGUE
Longitudinal cross-section of head:left view
Biochemical Analysis:
C # Biochemical homeostasis
Vitamin B1 (thiamine)    D=0.733    E=4
Follicle-stimulating hormone  D=0.759
```

Fig.64.

In this report the meaning of these values can read as we introduce before.
E value meaning is different in Entropy analysis and NLS analysis.

NLS diagnostic and therapy

The report has two models, show you in the following:

Date	Research	Standards	Variance	Entropy
2015/11/10	Longitudinal cross-section of head:left view	Follicle-stimulating hormone	0.759	-1
2015/11/10	Longitudinal cross-section of head:left view	Vitamin B1 (thiamine)	0.733	4

EXIT

Update

Report

Export to RTF

Edit report

☒ Print group etalon ☒ Print image group ☒ Print image name ☐ Print description

BASIC CATALOGUE

Longitudinal cross-section of head:left view

Biochemical Analysis:

C # Biochemical homeostasis

Vitamin B1 (thiamine) D=0.733 E=4

Follicle-stimulating hormone D=0.759

Report 2

Export to PDF

Edit Report 2

Fig.65

Results of Non-Linear Analysis System				
Name	wer es we			
Birthday	1975/1/1	Age	40	Phone
Address				
Comment				
				Description
BASIC CATALOGUE				
Longitudinal cross-section of head:left view				
C # Biochemical homeostasis				
Vitamin B1 (thiamine)				D=0.733 E=4
Follicle-stimulating hormone				D=0.759 E=-1

Fig.66.

NLS diagnostic and therapy

Reprinter

Reprinter allows to put down the information about etalons on various carriers (Water, Alcohol, Sugar, Paraffin) - (Fig.67).

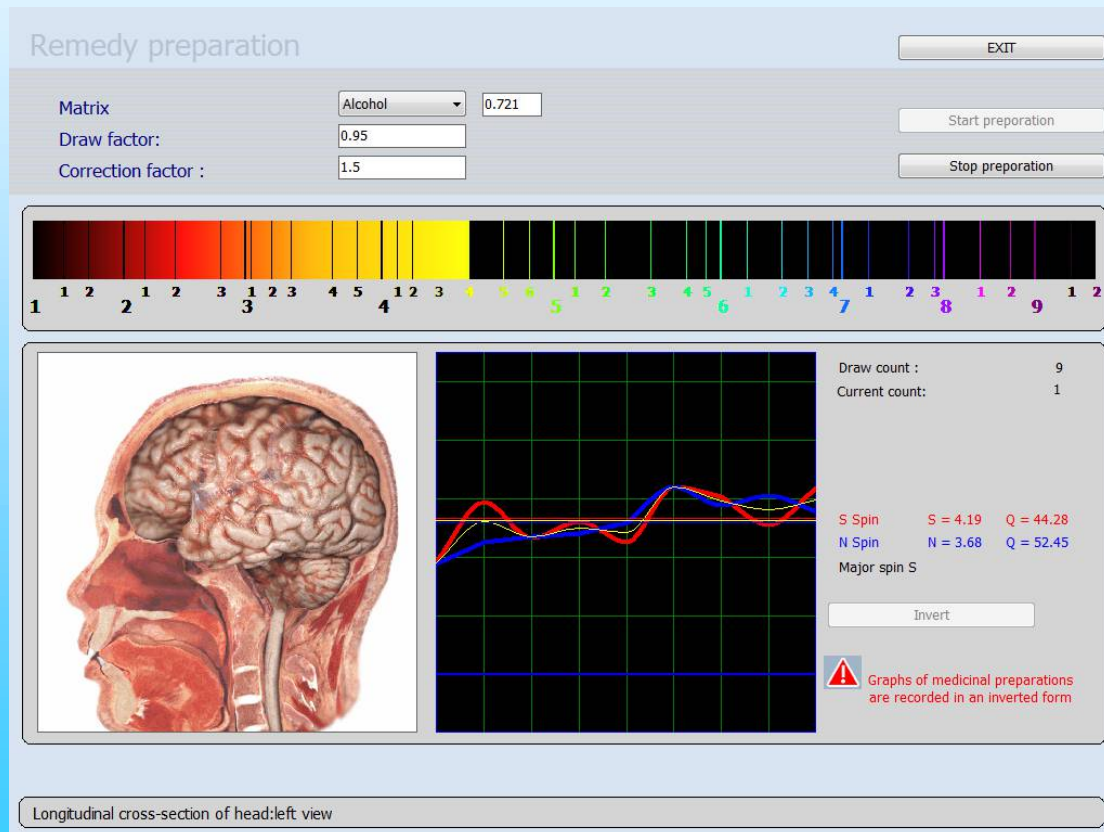


Fig.67.

NLS diagnostic and therapy

The function 'Reprint' also works along the principles of bio-resonance. A 'Reprint' is a 'copy' composed of frequencies at disposal in the database, frequencies specific to the organ treated. It is possible to charge a liquid with this Reprint of frequency. The client should absorb these frequencies during several weeks. When the liquid is charged, the frequencies are inverted, thus the opposite of the 'incorrect' measurements. It is thus possible to bring the functions of the organs towards frequencies approaching the structural frequencies (bringing the curves closer together).

To do this a glass has to be put into the resonance chamber, then click INVERT because the program contains inverted frequencies. Then select the type of carrier medium(water, alcohol, sugar, paraffin) and click START Preparation. The liquids suited to contain information are water, alcohol and paraffin, because they can retain and keep the frequencies during a long period.

NLS diagnostic and therapy

An other variation of the function 'Reprint', is the emission of various medication frequencies into the liquid. The given database contain frequencies of various alimentary additives, homeopathic formula, phyto and allopathic remedies, all placed in inverted form. It is possible to send (Reprint) these into a liquid in a manner identical with the organs. It is thus possible to arrive at an individual 'liquid solution' exclusive to this person.

It is possible to charge up to five different frequencies into the same bottle. The medication will find the organ appropriate to its resonance, which can be disturbed if there are more than five medications in use. The ideal would be to use a container for each organ, charged with only one frequency. Thus, if we want to treat the heart, the liver and the kidneys, the patient can have three different containers to be used individually at the time when the organ is most active according to the Chinese energetic hour clock. However, such a way to take the medicines is not always practical at the right moment, and it is then simpler and more polyvalent to charge all the frequencies into one bottle.

NLS diagnostic and therapy

Choose a necessary medicine effective for the given patient (index D < 0,425 = a medicine in the red zone) and click the button **Reprinter**. It is important to remember that all medicines are written down in a database in the inverted way, therefore before the record begins it is necessary to click the button **invert**. Then click **Start preparation**. For the urgent interruption of the process of manufacturing click the button **Stop preparation**. When the data recording on the carrier is finished, the program will stop automatically. To finish the work with Reprinter click the button **Exit**.

Efficiency of the given medicines differs depending on a matrix:

Water: For this purpose is advised to be used to cure acute processes. Preparation on the water is effective 2-3 weeks.

Alcohol: medicine made on the basis of it is effective up to 2-3 months.

Sugar: medicine on the basis of dairy is effective for 6-9 months and is used for treatment of chronic diseases. One dose of a medicine for acute processes usually make 4-8 drops or grains 3 times a day. For children under the age of 14 use 2-3 drops.

Paraffin: Medicine made on the basis of it is used for treatment of skin and neurologic diseases (eczema, radiculitis, neuralgia, etc)

NLS diagnostic and therapy

For treatment of chronic processes simultaneous record of several medicines (2-4) on one carrier is possible. For treatment of chronic processes the quantity of medicines can be increased to 6-8.

Attention! All materials (sugar, medicines, paraffin, etc) should be put into Reprinter papered or poured in a glass flask. Otherwise molecules of these substances may deposit in reprinter which can influence on the future results and worsen the effectiveness of medicine. Please wipe the **Reprinter** with a dry rag only and avoid water in it.

Print report

When you need to print report, you can click the '**Print researches**'

The screenshot shows a medical software interface with the following components:

- Form Fields:**
 - Last name: Black
 - Name: Tom
 - Middle name: Y
 - Age: 40
 - Sex: Male
 - Blood group: 0 0
 - Address: America
 - Phone: (empty)
- Buttons:**
 - New card
 - Select card
 - Print epicrisis
 - Save to disk
 - Print researches** (circled in red)
- Search and Actions:**
 - Search: (empty text box)
 - EXIT
 - Delete by date
 - Delete research
 - Delete file card
- Time and Reception:**
 - 15:33:53
 - Reception by Doctor
 - Time 15:33/0:00
- Research List:**

Date	Name of research
23.11.2015	Longitudinal cross-section of head:left view
23.11.2015	Longitudinal cross-section of head:left view (META-therapy)
24.11.2015	Horizontal thoracotomy at the level of the 6th thoracal vertebra
24.11.2015	Cross section of abdomen at the level of 1st lumbar vertebra
24.11.2015	Horizontal cross-section of trunk at the level of umbilicus
- Graphic and Analysis:**
 - Graphic: (Anatomical illustration of a human head and neck in cross-section)
 - Graphic
 - RESEARCH
 - View result
 - Comparative analysis

Fig.68.

Print report

Print Menu, The program allows to print the most effective etalons (Fig.69) chosen by the doctor during research.

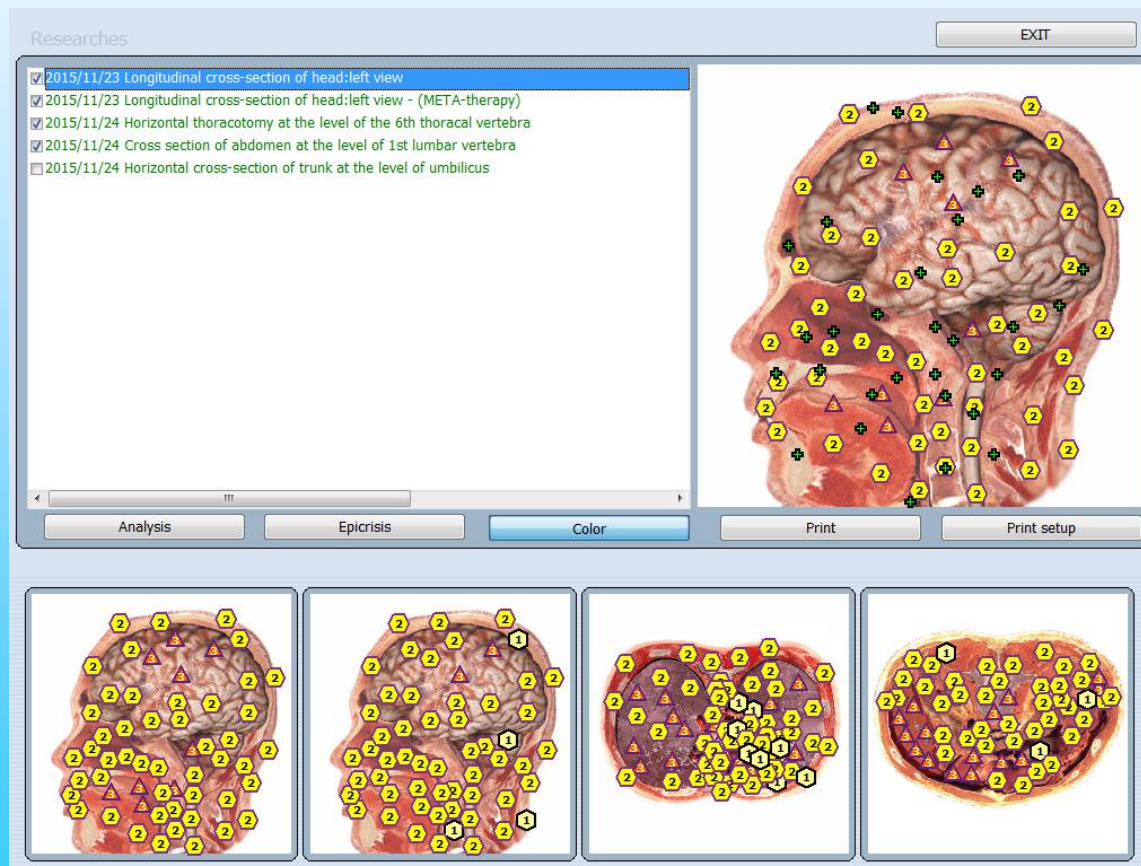


Fig.69.

Print report

Exit : back to Main menu .

Analysis : allows viewing of research results.

Epicrisis : to write down additional explanations for the patient and to look through the saved etalons. To print the results click on the button Print Epicrisis.

It is possible to add pictures with virtual models of up to four organs into print, just choose them from the list.

Color : to print colour images click on the button, otherwise the images will be printed in black-and-white.

Print : to start print click the button .

Print setup : to setup the print format

Backup

Saving the data.

If you click the button Save to disk in the Card file, you will enter a special menu (Fig.70) which allows to copy the data of the patient on a disk or to load the data from a disk into the program.

First it is necessary for you to choose one of the options at the top of the window: to load the data (Into programs) or to keep the data (From programs). The menu allows to save the data to any carrier such as: U disk, CD, Hard disk etc. Then you click the button Copy to disk (Copy from disk) depending on operation performed and the computer will suggest you to choose a folder for record.

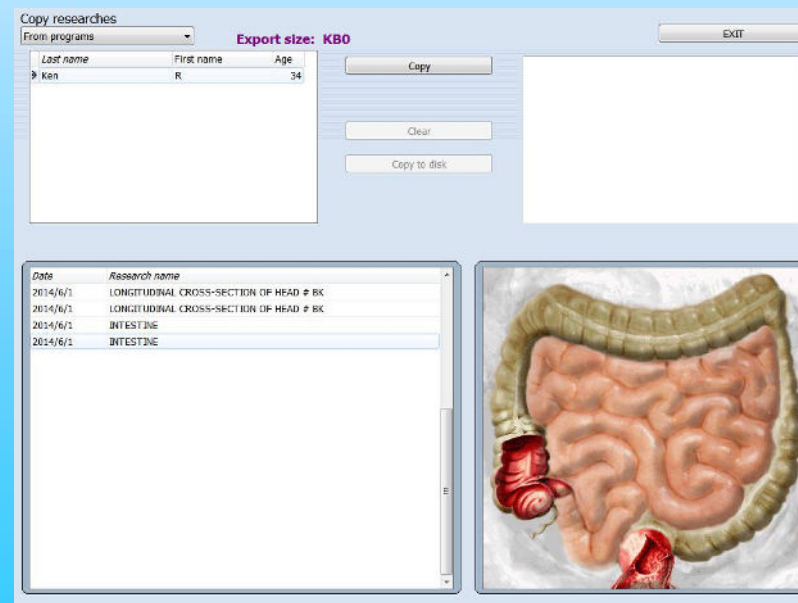


Fig.70.

Backup

Backup the patients database, Click '**Copy**' button(Fig.71).

Copy researches

From programs Export size: KB0 EXIT

Last name	First name	Age
Ken	R	34

Copy

Clear

Copy to disk

Date	Research name
2014/6/1	LONGITUDINAL CROSS-SECTION OF HEAD # BK
2014/6/1	LONGITUDINAL CROSS-SECTION OF HEAD # BK
2014/6/1	INTESTINE
2014/6/1	INTESTINE

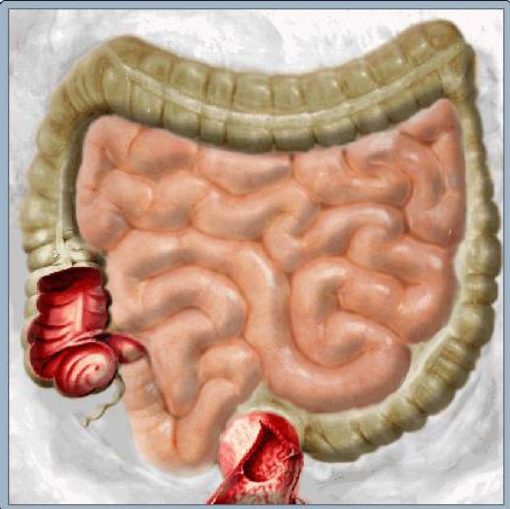


Fig.71.

Backup

Click '**Copy to disk**' button(Fig.72).

Copy researches

From programs

Export size: KB52

EXIT

Last name	First name	Age
Ken	R	34

Copy

Clear

Copy to disk

Ken R 34

Date	Research name
2014/6/1	LONGITUDINAL CROSS-SECTION OF HEAD # BK
2014/6/1	LONGITUDINAL CROSS-SECTION OF HEAD # BK
2014/6/1	INTESTINE
2014/6/1	INTESTINE

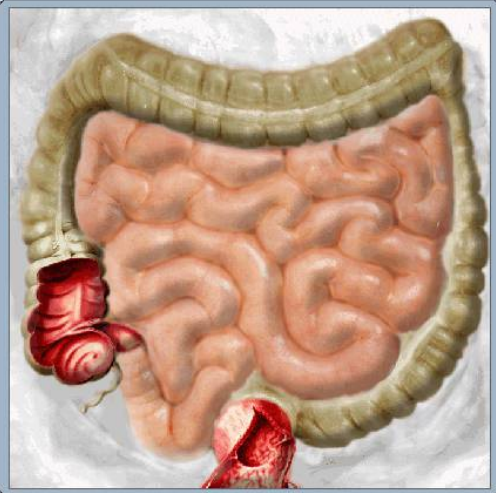


Fig.72.

Backup

Select save directory, Click '**OK**' button.(Fig.73).

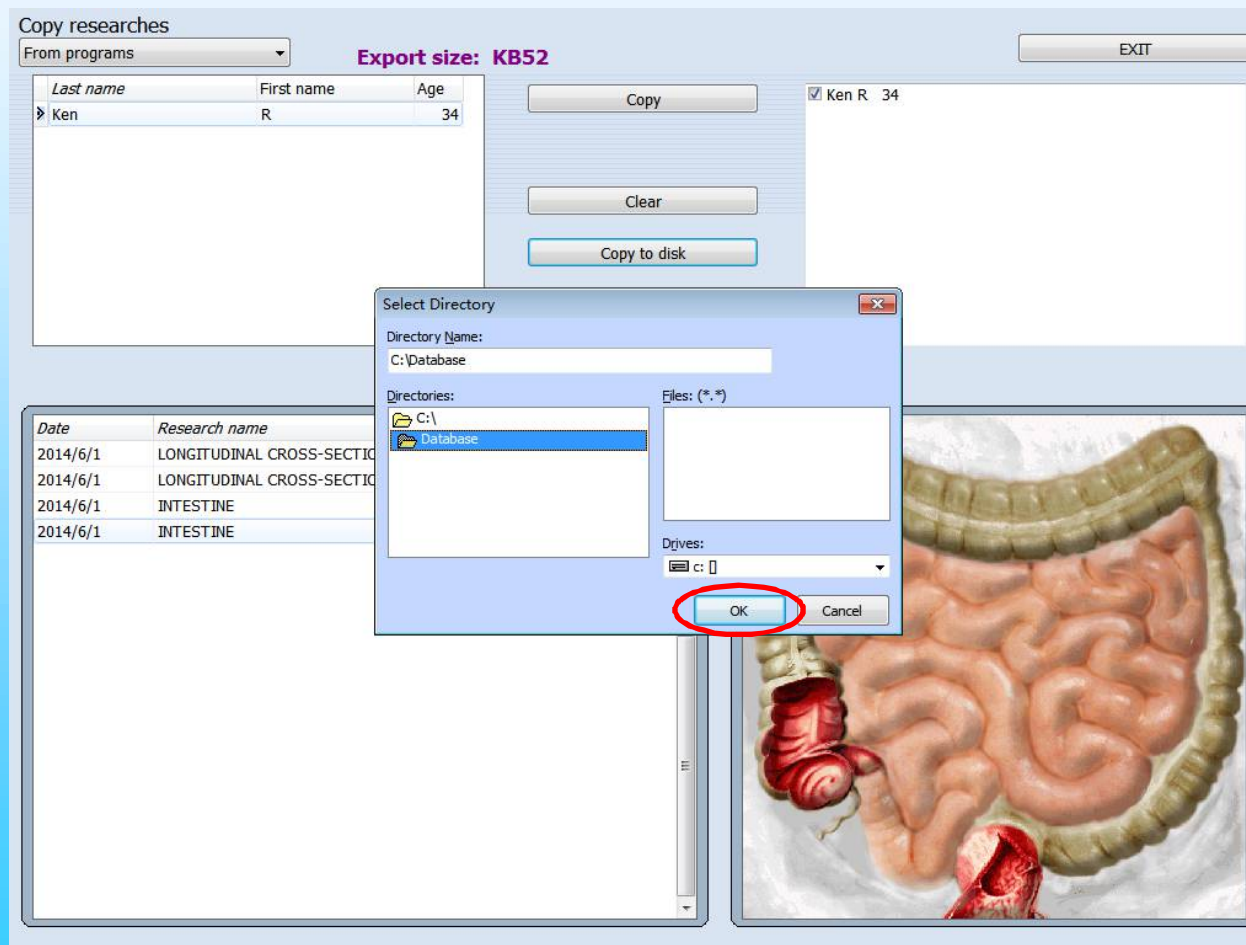


Fig.73.

Backup

Restore the patients database, First, select '**Into programs**' and select restore database file and Click '**OK**' button and Click '**Copy**' button.(Fig.74).

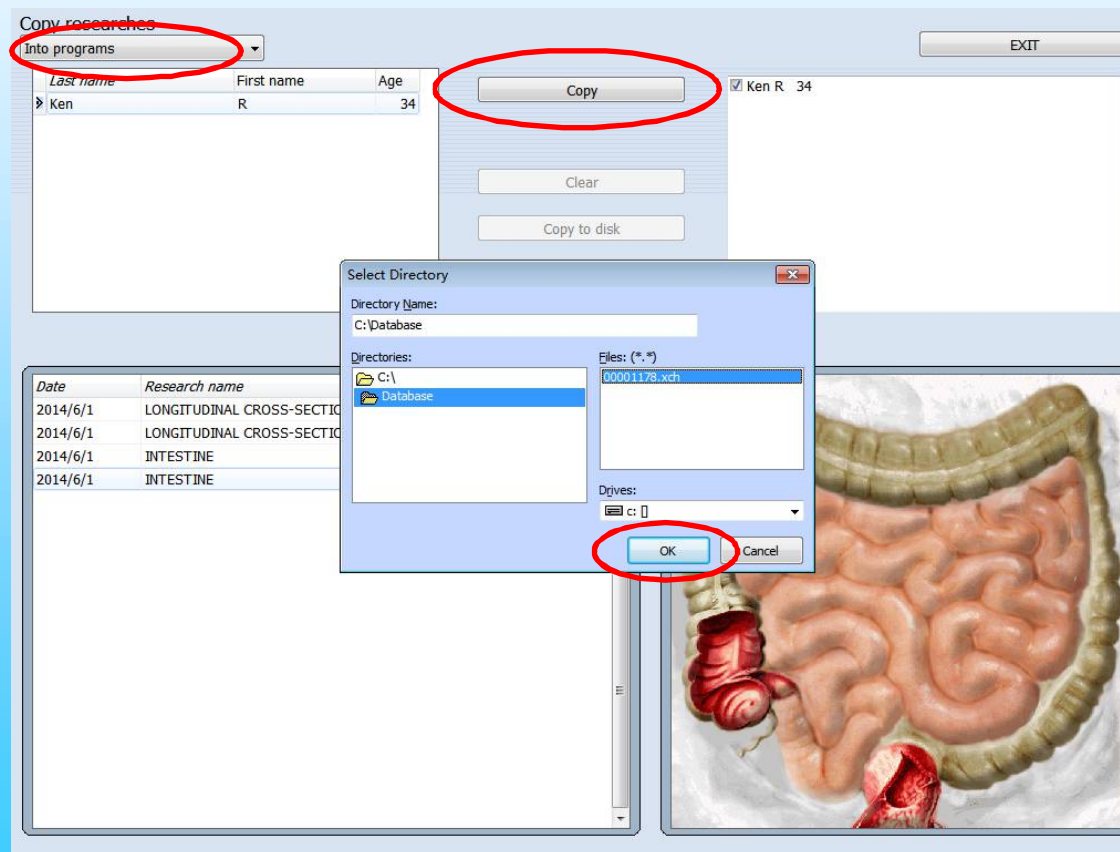


Fig.74.

Finish all the tests, then click the **'Exit'**

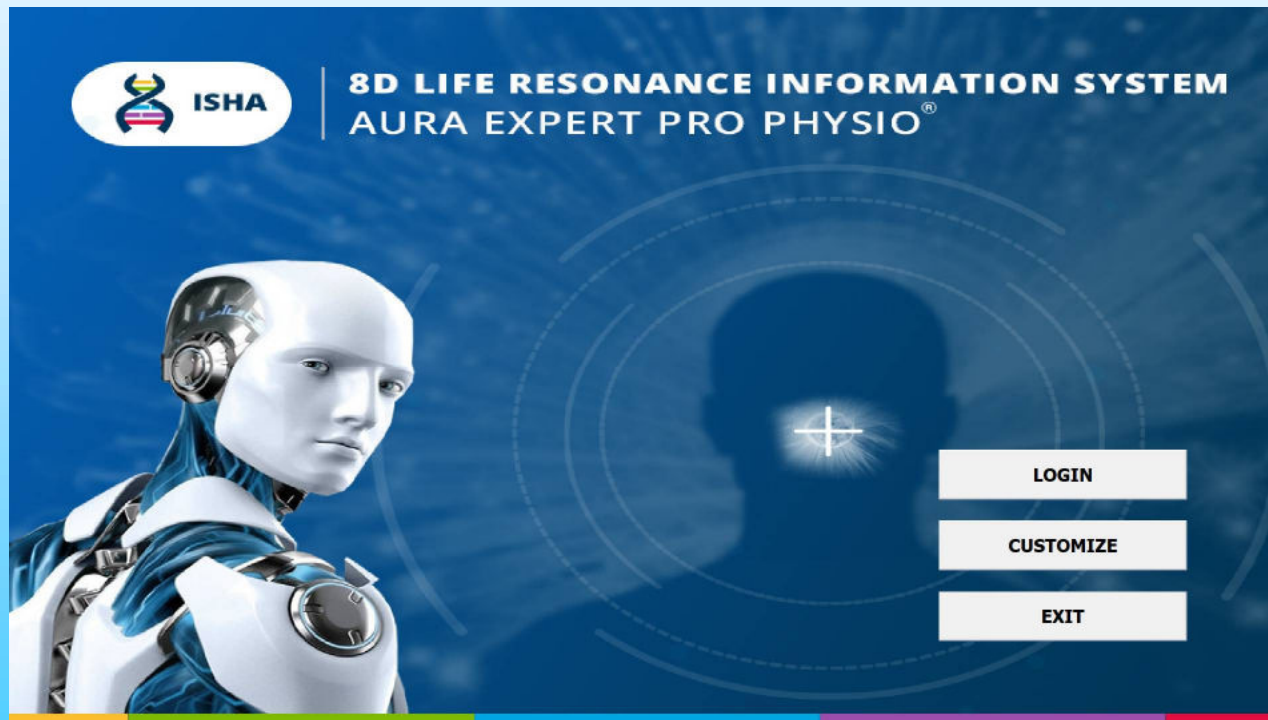


Fig.75.

Notice

- A. Participants should remove all metal objects, there are organs excision in advance.
- B. Detection process, the participants' hands and feet do not cross.
- C. A person the same organ do not test twice in a day.
- D. Long time no people to use, please be sure the machine is closed.
- E. Turn on the host machine 1 minute later can operat the software, it can protect the software database better.
- F. Wear Bio-inductor in correct way.
- G. Avoid using device under the strong light, it will affect the Bio-inductor work.
- H. Turn on/off machine in sequence.



ISHA



Instead of the biosensors you can take dna samples and do scans and treatments worldwide in the ISHA Quantum Meta Black Box. So that you HUMANS, DOGS, CATS, HORSES, can just walk around freely


Use hair, saliva, blood, nail parts, even a HQ small full body photo and put these in the ISHA QMBB (use a small crystal glass to put all in or a glass vial (s)

And you can do worldwide scans and treatment A big market ! Soo many clients to come !

[ISHA QMBB link](#)

We also advise the ISHA portable zapper to kill parasites, worms, fungi, helminths and lower their bio activity for dogs, horses, cats, cows, etc.



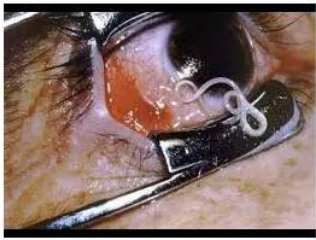

"We have a tremendous parasite problem right here in the United States. It is just not being addressed."

-Dr. Peter Wina, Chief of the Patho-Biology in the Walter Reed Army Institute of Research in 1991

Do you have any of these symptoms?
YOU MAY HAVE PARASITES

1 Diarrhea	7 Loss of appetite
2 Abdominal pain	8 Passing a worm in a stool
3 Weight loss	9 Stools containing mucus and blood
4 Fatigue	10 Rash or itching around the rectum
5 Gas or bloating	11 Restlessness or difficulty sleeping
6 Nausea/ vomiting	12 Dizziness



Ascaris lumbricoides worms passed by a child in 2007.

ISHA RIFE Adjustable POWER BUGS Zapper, powerfull killer of parasites and worms.

<https://nonlinearsystem.eu/shop/zappers-rifebob-beck-don-croft-isha/pre-order-within-1-july-accepted-isha-31-volts-adjustable-power-zapper-powerfull-deep-killer-parasites-worms-including-worldwide-free-shipping-finally-get-working-rife/>



For more information, visit the international global 170 countries members forum at www.ishaforum.com

Advice: **study the ISHA Apprentice Masters Classes** if you really want to know everything.

And start by reading the manual.

Also watch the **free videos on the forum** and youtube

[ISHA WEB SHOP](#)